

Shielding Design Methods for Linear Accelerators

Melissa Martin, MS, FACR, FAAPM, FACMP

Therapy Physics Inc., Gardena, CA 90248

Melissa@TherapyPhysics.com

AAPM 51st Annual Meeting

Anaheim, CA July 27, 2009

Key Messages in This Presentation

Page 2

- Each linear accelerator vault is unique
- Challenges in generating a shielding report
 - Identifying the locations around the vault that require a calculation
 - Appropriately calculating the shielded dose rate for these locations
 - Communicating the calculation implications to the architect and contractor
- Do not expect to generate a report simply by filling numbers in a spreadsheet
 - Assumptions implicit in spreadsheet may not match vault
 - Especially true if you do not understand the calculations in the spreadsheet
 - » Including how to adapt the calculations to the vault

Required Information for Shielding Designs


Page 3

- Architectural drawings of equipment layout in room
- Architectural drawings of surrounding areas indicating usage of these areas - offices, restrooms, corridor, exterior, etc.
- Elevation view of room or construction of floor and ceiling and distance between floors

Therapy Shielding Calculations Are Primarily Based on NCRP Report No. 151

Page 4

- Report Title: "Structural Shielding Design and Evaluation for Megavoltage X- and Gamma-Ray Radiotherapy Facilities"
 - Released December 31, 2005
- Calculations here illustrate the NCRP 151 recommendations
- Previous NCRP reports are also cited in some cases
 - e.g., NCRP 51 and NCRP 79



NCRP 151 recommendations are addressed throughout this presentation

Topics

Page 5

- Primary and Secondary Barriers
 - Simple primary barrier calculations, including required width
 - Secondary barrier calculations
 - » Photon leakage, neutron leakage, scatter, and IMRT impact
 - Laminated primary barrier calculations (i.e., barrier with metal)
 - Tapered ceilings
 - Lightly shielded wall for vault below ground level
- Vault entrances
 - Mazes (five examples with five different layouts)
 - Direct-shielded doors
- Skyshine
 - Photon and neutron skyshine for lightly-shielded ceiling
 - Generally not recommended for new construction
 - May be appropriate for cost-effective retrofit to existing vault

Linear Accelerator Energy

Page 6

- BJR #11 megavoltage (MV) definition used here
 - British Journal of Radiology (BJR) Supplement No. 11
- Comparison of BJR #11 and BJR #17 MV definitions

BJR #11 MV	4	6	10	15	18	20	24
BJR #17 MV	4	6	10	16	23	25	30

NCRP 151 Recommended Workload [1 of 2]

Page 7

- Workload (W)
 - "Time integral of the absorbed-dose rate determined at the depth of the maximum absorbed dose, 1 m from the source"
- 450 Gy/wk maximum weekly workload cited in NCRP 151
 - Kleck (1994)
 - » Maximum 350 Gy/wk for 6 MV
 - » Maximum 250 Gy/wk at high MV for dual energy
 - Mechalakos (2004)
 - » Maximum 450 Gy/wk for 6 MV single-energy
 - » Maximum 400 Gy/wk for dual energy
 - NCRP 151 Section 7 examples assume 450 Gy/wk at high MV

450 Gy / wk absorbed dose is the default weekly workload

NCRP 151 Recommended Workload [2 of 2]

Page 8

- 30 patients treated per day is default assumption
 - NCRP 151 default recommendation for busy facility
 - Can also base on a conservative estimate influenced by factors such as historical workload and demographics
 - » e.g. lower patient workload for facility in small town
- 3 Gy absorbed dose per patient treatment default
 - Assumption used in NCRP 151 Section 7 examples
 - Consistent with 450 Gy/wk with 30 patients treated per day
 - » 450 Gy/wk = 5 treatments/wk/patient x 3 Gy/treatment x 30 patients
 - Equivalent to 219 cGy treatment fraction (0.73 tissue maximum ratio)
 - » Intentionally somewhat conservative (compared to ~200 cGy fraction) since no specific allowance for quality or maintenance workload
 - Can be based on direct knowledge of accelerator use instead
 - » But preferable to stick with the NCRP 151 default

450 Gy/wk is consistent with 30 patients & 3 Gy/treatment

Workload Assumptions for Dual Energy Linear Accelerators

Page 9

- Preferable to assume full 450 Gy/wk workload is at the higher energy
 - Simpler, more conservative calculation
 - Appropriate for new construction
- For existing construction, dual-energy calculation may be appropriate
 - If modifications to existing vault are difficult and size constrained
 - Split 30 patient workload to ensure at least 250 Gy/wk at higher MV
 - » With 17 patients, 255 Gy/wk at higher MV

Mode	Gy/wk/patient	Patients/day	W (Gy/wk)
Single x-ray mode	15	30	450
Dual x-ray mode	15	30	450
High-X mode	15	17	255
Low-X mode	15	13	195

At least 250 Gy/wk at high MV mode

Radiation Protection Limits

Page 10

- Shielding Design Goal (P)
 - Level of dose equivalent (H) used in the design calculations
 - Applies to barriers designed to limit exposure to people
 - » Limiting exposure to unoccupied locations is not the goal
 - Stated in terms of mSv at the point of nearest occupancy
- Recommended values for shielding design goal
 - 0.10 mSv/week for controlled areas
 - 0.02 mSv/week for uncontrolled areas
- Typical international shielding design goals
 - 0.12 mSv/week for controlled areas
 - 0.004 mSv/week for uncontrolled areas

Controlled Areas

Page 11

- Limited-access area in which the occupational exposure of personnel to radiation or radioactive material is under the supervision of an individual in charge of radiation protection
- Access, occupancy and working conditions are controlled for radiation protection purposes
- Areas are usually in the immediate areas where radiation is used, such as treatment rooms and control booths, or other areas that require control of access, occupancy, and working conditions for radiation protection purposes
- The workers in these areas are those individuals who are specifically trained in the use of ionizing radiation and whose radiation exposure is usually individually monitored

Uncontrolled Areas

Page 12

- All other areas in the hospital or clinic and the surrounding environs
- Trained radiation oncology personnel and other trained workers, as well as members of the public, frequent many areas near controlled areas such as examination rooms or restrooms
 - Choice of appropriate occupancy factors ensures the protection of both those who are occupationally exposed as well as others who might be exposed in these areas

Radiation Protection Limits for Locations

Page 13

- Protected location
 - Walls: 1 ft beyond the barrier
 - Ceilings: 1.5 ft above the floor of the room above the vault
 - Floors: 5.5 ft above the floor of the room below
- Permissible dose at protected location depends on occupancy
- Occupancy factor (T):
 - Fraction of time a particular location may be occupied
- Maximum shielded dose rate at protected location: P/T
 - Assuming occupancy factor T for protected location

Max shielded dose rate traditionally referred to as P/T

NCRP 151 Recommended Occupancy

Page 14

- T=1: Areas occupied full-time by an individual) e.g. administrative or clerical offices; treatment planning areas, treatment control rooms, nurse stations, receptionist areas, attended waiting rooms, occupied space in nearby building
- T = 0.5: Adjacent treatment room, patient examination room adjacent to shielded vault
- T = 0.2: Corridors, employee lounges, staff rest rooms
- T = 0.125: Treatment vault doors
- T = 0.05: Public toilets, unattended vending rooms, storage areas, outdoor areas with seating, unattended waiting rooms, patient holding areas, attics, janitor's closets
- T = 0.025: Outdoor areas with only transient pedestrian or vehicular traffic, unattended parking

Occupancy Factor Selection

Page 15

- For interior locations, T=1 and T=0.2 are most common
 - T = 1 for work locations
 - T = 0.2 for locations not occupied continuously
- For exterior locations, T = 0.05 is most common
- T < 1 now appropriate for some controlled locations
 - Use with T = 0.125 for vault entrance with caution; any higher occupancy location further away must also be protected
 - T = 0.5 for adjacent vault appears to be reasonable assumption
- Select T = 0.05 for interior locations with caution
 - Should be very unlikely to be occupied (storage, attic, closets)
- T = 0.025 for exterior locations with restricted access
 - NRC hourly limit is more constraining for unrestricted locations

Use Factor

Page 16

- Use Factor (U) is the fraction of the workload for which the primary beam is directed at the barrier in question
- Traditionally U = 0.25 for lateral barriers, ceiling, & floor
- U = 0.1 for tapered portions of ceiling barrier (Example 11)
- Applies to primary barrier calculations, usually not secondary
- NCRP 151 Table 3.1 below consistent with these values
 - TBI may require deviation from these values

90° gantry angle intervals

Angle Interval Center	U (percent)	Standard Deviation (percent)
0° (down)	31.0	3.7
90° and 270°	21.3 (each)	4.7
180° (up)	26.3	3.7

45° gantry angle intervals

Angle Interval Center	U (percent)	Standard Deviation (percent)
0° (down)	25.6	4.2
45° and 315°	5.8 (each)	3.0
90° and 270°	15.9 (each)	5.6
135° and 225°	4.0 (each)	3.3
180° (up)	23.0	4.4

Hourly Limit for Uncontrolled Areas

Page 17

- Recommendation is based on maximum Time-Averaged Dose Equivalent Rate (TADR) per hour (NCRP 151, 3.3.2)
 - TADR synonymous with shielded dose rate in this presentation
- Calculation adjusts weekly TADR (R_w) to hourly TADR (R_h)

$$R_h = (M/40) R_w$$
 - where M = ratio of maximum to average patient treatments per hour
 - Shielding must be sufficient so that $R_h \leq 0.02$ mSv/wk NRC limit
- More realistic than traditional U=1 recommendation
 - Several beam orientations are almost always used for each patient
 - Exception: 35 Gy/hr with U=1 for a lateral barrier used for TBI

NCRP 151 eliminates traditional U=1 assumption

Hourly Limit for Uncontrolled Areas: Recommended Approach

Page 18

- Max patients / hour at highest energy: Six
 - Maximum in any one hour estimated as one each 10 minutes
 - Max workload per hour (W_h) is 6 patients x 3 Gy/patient = 18 Gy
- Max weekly P/T (mSv/wk) = 0.02 (mSv/hr) W (Gy/wk) / W_h (Gy/hr)
 - where W = 450 Gy/wk (single/dual) or W=255 Gy/wk (at high MV)

Mode	Patients per day	W (Gy/wk)	Max Patients per hour	Gy per Patient Treatment	Max Gy/hr (W_h)	Weekly Max P/T (mSv/wk)	Equiv. Min T
Single MV mode	30	450	6	3	18	0.500	0.040
Dual MV mode	30	450	6	3	18	0.500	0.040
High MV mode	17	255	6	3	18	0.283	0.071
Low MV mode	13	195	(High MV)	3	18		

Max P/T applies to both primary & secondary barriers

- Minimum occupancy (T) = W_h (Gy/hr) / W (Gy/wk)
 - Hourly NCR limit and weekly NCRP 151 limit are both 0.02 mSv
 - Implies full benefit of T=0.025 applies only to restricted locations

Page 19

Primary Barrier Photon Shielded Dose Rate

- Photon unshielded dose rate

$$H_{pri} = \frac{WU}{d_{pri}^2}$$
 where distance is in meters
- Transmission by shielding material thickness t

$$Trans. = 0.1 \times 10^{[-(t - TVL_1)/TVL_2]}$$
 - Where TVL_1 and TVL_2 are the values for the first and subsequent tenth-value layers, respectively
 - Assumes $t > TVL_1$
- Shielded dose rate is unshielded dose rate times transmission
 - Must be less than P/T

Page 20

Table 1: NCRP 151 Table B.2 Primary Barrier Photon TVLs (mm)

Linac MV	Lead		Concrete		Steel		Earth		Borated Poly	
	TVL1	TVL2	TVL1	TVL2	TVL1	TVL2	TVL1	TVL2	TVL1	TVL2
4	57	57	350	300	99	99	549	470	866	743
6	57	57	370	330	100	100	580	517	916	817
10	57	57	410	370	110	110	643	580	1015	916
15	57	57	440	410	110	110	690	643	1089	1015
18	57	57	450	430	110	110	705	674	1114	1064
20	57	57	460	440	110	110	721	690	1138	1089
25	57	57	490	460	110	110	768	721	1213	1138

Estimated by density vs. concrete
 concrete = 2.35 g/cm³ [NCRP 151, p. 69]
 earth density = 1.5 g/cm³ [NCRP 151, p. 72]
 borated poly = 0.95 g/cm³ [NCRP 151, p. 162]

NCRP 151
Table B.2

Include density in the shielding report and recommend that construction contracts specify the density

Page 21

TVLs for Other Material

- High density concrete
 - Alternative to lead / steel if wall must have limited thickness
 - Generally construction uses blocks instead of poured concrete
 - Mixers not designed for use with high density aggregates
 - Photon TVL based on density relative normal concrete 147 lb/ft³
 - Typically 288 lb/ft³ for primary barriers, 240 lb/ft³ secondary
 - Neutron TVL considered to be the same as normal concrete
 - With boron added to compensate for lower hydrogen content
- Conventional concrete block
 - Generally less than 147 lb/ft³ density, so adjust TVLs accordingly
- Asphalt may provide ceiling shielding
 - Parking lot placed over top of vault
 - Typical density is 2.0 g/cm³
 - Resulting in TVL 1.18 times concrete TVL

Page 22

Typical Primary Concrete Barrier

- Primary barrier calculation tends to be relatively accurate
 - Unlike secondary barrier calculation, which tends to be conservative
- Desirable to have factor of 2 or 3 margin for shielded dose rate to account for variation in concrete density
 - NCRP 151 factor of 2.7 for primary barriers with metal above 10 MV is reasonable goal for all primary barriers
- Typical concrete primary barrier thickness (ft)

P/T	6 MV	18 MV
0.02	6.5	8
0.1	6	7.5
0.2	5.5	7
0.4	5	6.5 to 7
0.8	4.5 to 5	6
- Shielding report should emphasize that construction contracts specify 147 lb/ft³ concrete density

Page 23

Factor of 2 to 3 Margin Recommended for Primary Shielded Dose Rate Calculation

- 2.7 margin recommended for laminated barriers by NCRP 151
 - Based McGinley & Butker (1994)
 - Attributed to capture gammas
- Safety survey vs. calculated dose rate indicates factor 2 to 3 appropriate for all primary barriers
 - Likely due to variation in concrete density, not capture gammas
- 2.7 recommended by NCRP 151 for laminated barriers is appropriate goal for all barriers

Line	Photon Dose Equivalent Rate (nSv/h)		
	Calculated	Measured	Meas / Calc.
a	27.5	55.6	2.0
b	3.3	3.3	1.0
c	11.6	31.1	2.7
d	1.9	1.9	1.0
e	168.3	244.0	2.3
f	5.8	6.7	1.1

Line	Protected Location	P/T	Shielded Dose (mSv/wk)		
			Calc.	Meas.	Ratio
a	Toilet	0.080	0.042	0.009	0.2
b	Toilet	0.080	0.037	0.009	1.9
c	Adjacent Vault	0.100	0.031	0.024	0.8
d	Adjacent Vault	0.100	0.034	0.031	0.9
e	Adjacent Vault	0.100	0.031	0.031	1.0
f	Adjacent Vault	0.100	0.022	0.042	1.9
g	Adjacent Vault	0.100	0.039	0.100	2.6
h	Exterior Wall	0.165	0.115	0.115	1.0
i	Exterior Wall	0.165	0.034	0.069	2.1
j	Exterior Wall	0.165	0.031	0.076	2.5
k	Ceiling	0.320	0.136	0.122	0.9

Line	Protected Location	P/T	Shielded Dose (mSv/wk)		
			Calc.	Meas.	Ratio
a	Office	0.020	0.006	0.003	0.5
b	Ceiling	0.165	0.008	0.005	0.7
c	Ceiling	0.320	0.116	0.139	1.2

Page 24

Directly Solving for Barrier Thickness

- NCRP 151 typically illustrates calculations by solving for the required thickness instead of directly calculating time-average dose rate
- Transmission factor B_{pri}
 - Reciprocal of required attenuation
$$B_{pri} = \frac{P d_{pri}^2}{WU T}$$
- Number of tenth-value layers (TVLs): $n = -\log_{10}(B_{pri})$
- Required barrier thickness

$$t_c = TVL_1 + (n-1) TVL_2$$

“Two Source Rule”

Page 25

- Applicable when required thickness is calculated for more than one type of radiation
- If thickness required is comparable for two types of radiation, add 1 HVL to the larger thickness
- If the two thicknesses differ by a tenth-value-layer (TVL) or more, the larger barrier thickness is used
- Also sometimes called the “Add HVL Rule”

Examples At End of Presentation Use Time Averaged Dose Rate Instead of Calculating Thickness


Page 26

- Two Source Rule either over-estimates or under-estimates required shielding for two or more sources of radiation
- Up to three types of radiation for secondary calculations
- TADR must be calculated anyway for primary barriers
 - To determine factor of 2.7 margin
 - TADR needed for hourly limit
- Potentially multiple layers of dissimilar material in barrier
- No direct way to calculate required thickness for photon neutron generation

Primary Barrier Width

Page 27


- 1 foot margin on each side of beam rotated 45 degrees
 - Barrier width required assuming 40 cm x 40 cm field size
$$w = 0.4\sqrt{2} d_N + 0.6 \text{ m} \quad (\text{where } d_N \text{ is in meters})$$
- Field typically not perfectly square (corners are clipped)
 - 35 cm x 35 cm field size used to account for this

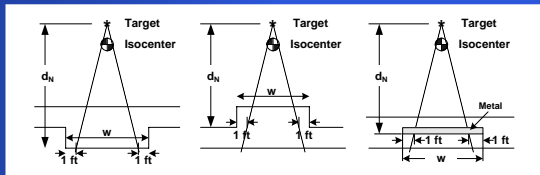

Primary Barrier Width Typically Calculated Assuming 35 cm x 35 cm Field Size

Page 28

- Field typically not perfectly square (corners are clipped)
 - 35 cm x 35 cm field size used to account for this
- $$w = 0.35\sqrt{2} d_N + 0.6 \text{ m} \quad (\text{where } d_N \text{ is in meters})$$

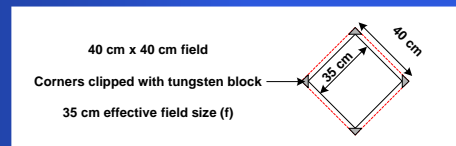

Secondary Barrier Photon Leakage

Page 29

- Leakage unshielded dose rate

$$H_L = \frac{W \times \text{leakage fraction}}{d_{sec}^2}$$
 - Assumes H_a in Sv and W in Gy
 - 0.1% leakage fraction is customary
 - Secondary distance d_{sec} in meters
- Calculate shielded dose rate using TVLs in NCRP 151 Table B.7
- Calculation tends to be conservative
 - Typical leakage 5X or more lower than 0.1% requirement
 - Unlike primary barriers, generally no need for extra margin




Table 2: Leakage TVLs (mm)

Page 30

Linac MV	Lead		Concrete		Steel		Earth		Borated Poly	
	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe
4	57	57	330	280	96	96	517	439	817	693
6	57	57	340	290	96	96	533	455	842	718
10	57	57	350	310	96	96	549	486	866	767
15	57	57	360	330	96	96	564	517	891	817
18	57	57	360	340	96	96	564	533	891	842
20	57	57	360	340	96	96	564	533	891	842
25	57	57	370	350	96	96	580	549	916	866

NCRP 151 Primary TVL Table B.2
 NCRP 151 Table B.7
 Varian TVL ratio relative concrete
 Est. by density vs. concrete
 concrete = 2.35 g/cm³ [NCRP 151, p. 69]
 earth density = 1.5 g/cm³ [NCRP 151, p. 72]
 BPE = 0.95 g/cm³ [NCRP 151, p. 162]

Note: NCRP 51 Figure E.14 indicates lead TVL is maximum near 6 MeV, so using primary TVL for leakage is reasonable

No data in NCRP 151 for steel leakage TVL.
 NCRP 51 Figure E.13 implies steel leakage TVL should be less than primary.
 Rationale for 96 mm steel TVL based on Varian document #12004 on next chart.

Conservative Leakage TVL for Steel: 96 mm

Page 31

Leakage TVLs from Varian Document #12004

- Concrete leakage TVLs slightly less than NCRP 151
- Steel TVL calculated from ratio in Varian Document

MV	TVL (mm)		Ratio
	Concrete	Steel	
6	280	88	3.2
10	320	91	3.5
15	330	89	3.7
18	330	89	3.7
25	360	90	4

From <http://www.varian.com/sharedcontent/pub/12004.pdf>

Varian ratio applied to NCRP 151 concrete leakage TVLs

- Average TVL = $(TVL_1 + 2 TVL_2) / 3$
 - Secondary barrier has at least 3 TVLs
- Average TVL between 89 and 96 mm
 - Calculated TVL varies since concrete TVLs rounded to cm
- 96 mm upper bound steel leakage TVL

MV	Concrete		Varian Ratio	Steel Calculated		
	TVL ₁	TVL ₂		TVL ₁	TVL ₂	TVL Ave
6	340	290	3.2	106	91	96
10	350	310	3.5	100	89	92
15	360	330	3.7	97	89	92
18	360	340	3.7	97	92	94
25	370	350	4	93	88	89

Leakage TVLs from 2007 Summer School*

Page 32

Tenth Value Layers

Primary TVLs (cm)**						
Energy (MV)	4	6	10	15	18	20
Concrete	35(28)	37(33)	41(37)	44(41)	45(53)	46(44)
Steel	9.8	10	11	11	11	11
Lead	5.7	5.7	5.7	5.7	5.7	5.7

Leakage TVLs (cm)**

Energy (MV)	4	6	10	15	18	20
Concrete	33(28)	34(29)	35(31)	36(33)	36(34)	36(34)
Steel**	8	8.5	8.7	8.7		
Lead**	4.5	4.6	4.7	4.7		

* First term is 1st TVL and term in brackets is for all other TVLs.
 ** Data from NCRP 4511
 ** Data from McShine

AAPM Summer School - July 28, 2007

* Peter Biggs, Primary & Secondary Composite Wall Materials, 2007 AAPM Summer School (Slide # 4)

- Caution: Pat McGinley at 2007 AAPM Summer School used a lead leakage TVL of 6.1 cm for a direct-shielded door example (not the 4.7 cm TVL above)

Table 2 lead & steel TVLs may be somewhat conservative

Intensity Modulated Radiation Therapy (IMRT)

Page 33

- IMRT requires increased monitor units per cGy at isocenter
 - IMRT ratio is the ratio of MU with IMRT per cGy at isocenter
- Percent workload with IMRT impacts shielding
 - 50% typically assumed; 100% if vault is dedicated to IMRT
- Account for IMRT by multiplying workload by IMRT factor
 - IMRT Factor = % IMRT x IMRT ratio + (1 - % IMRT)
- Leakage Workload: $W_L = W \times \text{IMRT Factor}$
 - W_L replaces W in leakage unshielded dose calculation with IMRT
- Lower IMRT factor appropriate for neutrons if calculate shielding at the higher MV for a dual MV machine

Table 3: IMRT Ratio Typical Values

Page 34

Manufacturer	IMRT Ratio	Percent IMRT	IMRT Factor	
			Photon	Neutron
Varian	3	50%	2	1
Siemens	5	50%	3	1.5
NOMOS	10	50%	5.5	2.75
Tomotherapy	16	100%	16	NA

- Typically assume 50% of treatments with IMRT
 - Pessimistic assumption for dual energy machine since most IMRT done at lower energy (e.g., >75% at 6 MV, <25% at 18 MV)
- Neutron IMRT factor (applicable to dual energy) assumes IMRT equally at high and low energy
 - Since most IMRT is done at the lower energy, an even lower neutron IMRT factor may be appropriate

IMRT Factor Calculation

Page 35

Calculation for single MV

Line	Parameter	Units	Single MV	Calculation
a	IMRT Ratio	MU/cGy	3	Varian
b	Fraction with IMRT	Ratio	0.5	Typical
c	IMRT Factor	Ratio	2	$a * b + (1 - b)$

- Calculation for dual MV
 - Shielded dose rate calculated separately at each MV
 - Including appropriate % IMRT at each MV
 - Total shielded dose rate is total at the separate MVs
 - Generally appropriate only for retrofit
 - marginal shielding, expensive and difficult to modify
 - Calculation at single (highest) MV recommended for new construction

Secondary Shielding for High Energy Linacs

Page 36

- May need to consider neutron leakage as well as photons
 - Not necessary if barrier consists solely of concrete
 - Is necessary for thin barrier containing significant metal
 - e.g., door or laminated barrier
- Calculation is of the same form as photon leakage calculation
 - But with different leakage fraction and TVLs
- Shielding typically calculated only at higher energy for dual energy linacs
 - Easier calculation than performing separate calculations for the two energies

Neutron IMRT Factor Calculation

Page 37

- IMRT factor lower for neutrons than photons for dual MV
 - Typically split between low and high energy for dual MV machine
 - Neutrons not produced below 10 MV
- Typical: 50% High-X & 50% Low-X with 50% IMRT at each MV
 - Conservative since far more IMRT at 6 MV than at 15 or 18 MV
 - Neutron IMRT factor 1 with these conservative assumptions
- Neutron Leakage Workload: $W_{Ln} = W \times \text{Neutron IMRT Factor}$

Line	Parameter	Units	Photon		Neutron		Calculation
			Low-X	High-X	Low-X	High-X	
a	IMRT Ratio	MU/cGy	3	3	0	3	Varian
b	Fraction with IMRT	Ratio	0.5	0.5	0.5	0.5	Typical
c	IMRT Factor per MV	Ratio	2	2	0	2	$a \cdot b + (1 - b)$
d	Fraction at each MV	Ratio	0.5	0.5	0.5	0.5	Expected usage
e	IMRT Factor * Fraction	Ratio	1	1	0	1	$c \cdot d$
f	IMRT Factor	Ratio	2		1		Sum Line e

NCRP 151 Neutron Leakage

Page 38

- Neutron leakage unshielded dose rate

$$H_n = \frac{W_{Ln} \times H_o}{(d_{sec} / 1.41)^2}$$

- H_n in Sv and W_{Ln} in Gy
- d_{sec} is secondary distance from isocenter to protection location (in meters)

- H_o from Table B.9 of NCRP 151

- Normalized at 1.41 meters from isocenter
- Leakage data in NCRP 151 is for older machines
- Best to use manufacturers' data for newer machines (next chart)

NCRP 151 Table B.9

Vendor	Model	MV	H_o @1.41 m mSv/Gy
Varian	1800	18	1.02 to 1.6
	1800	15	0.79 to 1.3
	1800	10	0.04
	2100C	18	
	2300CD	18	
Siemens	2500	24	
	KD	20	1.1 to 1.24
	KD	18	
	MD	15	0.17
	MD2	10	
Philips/ Elekta	Primus	15	
	SL25	25	2
	SL20	20	0.44
GE	SL20	18	
	SL25	18	
	Saturne41	12	0.09
	Saturne41	15	0.32
	Saturne43	18	0.55
	Saturne43	25	1.38

Table 4: Neutron Leakage Fraction

Page 39

- Neutron leakage unshielded dose rate

$$H_n = \frac{W_{Ln} \times H_o}{d_{sec}^2}$$

- H_n in Sv and W_{Ln} in Gy
- H_o is neutron leakage dose equivalent fraction normalized to 1 m from target

- H_o in Table 4 normalized to 1 m
 - Varian* and Siemens** values based on manufacturer data
 - Elekta data from Site Planning Guide***
 - GE data based on NCRP 151 Table B.9 normalized to 1 m

Vendor	MV	H_o @1 m Sv/Gy
Varian	10	4.0E-05
	15	7.0E-04
	18	1.5E-03
	20	1.9E-03
	24	2.0E-03
Siemens	10	2.0E-05
	15	4.2E-04
	18	9.9E-04
	20	1.4E-03
Elekta	10	3.0E-04
	15	7.0E-04
Philips	18	1.5E-03
	20	2.0E-03
GE	24	3.0E-03
	12	1.8E-04
	15	6.4E-04
	18	1.1E-03
	25	2.7E-03


* Varian: <http://www.varian.com/osup/pdf/12000.pdf> [Page 12, Average of 4 positions]

** Siemens: Conservative neutron leakage dose rates in patient plane with Q=10

*** Elekta: Nisy Ipe, "Neutron Shielding Design and Evaluations", 2007 AAPM Summer School


NCRP 151 Cites Figure A.2 (from NCRP 51) as Basis for Neutron TVL

Page 40

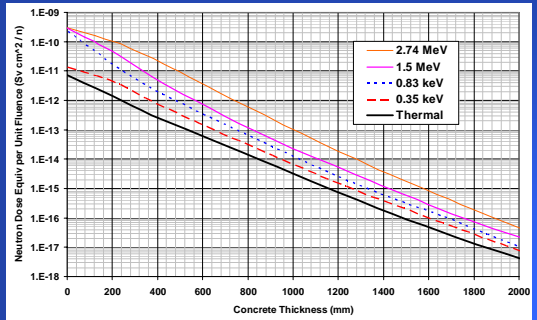

NCRP 151 Figure A.2 Normalized to Maximum Fluence

Page 41

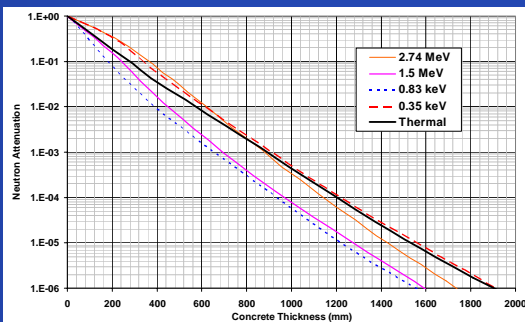

Neutron Leakage TVL Recommendation

Page 42

- TVLs based on Figure A.2 are somewhat inconsistent

- Curves originally in NCRP 51

- NCRP 151 recommends 250 mm as "conservatively safe estimate of the TVL_n"

TVL #	Cumulative Concrete Neutron TVLs				
	Thermal	0.35 keV	0.83 keV	1.5 MeV	2.7 MeV
1	277	337	176	246	367
2	286	307	193	226	312
3	296	304	217	232	295
4	301	305	232	243	286
5	307	312	243	256	286

Recommendation for laminated primary barriers, neutron leakage not specifically addressed

- TVL recommendation based on NCRP 79

- TVL_n = 155 + 56 * Neutron MV for concrete
 - 211 mm at 1 MV is traditional neutron leakage TVL for concrete
- TVL_n = 62 + 34 * Neutron MV for borated polyethylene (BPE)
 - 96 mm at 1 MV is traditional neutron leakage TVL for BPE
- Estimate other material from concrete or BPE based on hydrogen content
- Lead and steel provide negligible neutron attenuation

MV	Concrete		Earth		Borated Poly		Application
	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	
1	211	211	331	331	96	96	Leakage

Continuing to use the NCRP 79 neutron leakage TVLs is recommended

Page 43

Neutron TVLs for Other Material

- Concrete of varying density
 - Neutron density for high density concrete assumed the same as for normal weight concrete
 - High density concrete has slightly lower hydrogen content than normal concrete
 - High density concrete typically has boron added to maintain same neutron TVL as normal concrete
 - TVL for light concrete adjusted based on density like photon TVL
 - Likely a conservative assumption
- Asphalt has high hydrogen content
 - Same TVL as borated polyethylene assumed
 - e.g., McGinley reports 10 cm neutron skyshine TVL due to asphalt, which is comparable to primary BPE TVL

Page 44

Secondary Barrier Patient Scatter

- Patient scatter unshielded dose rate

$$H_{ps} = \frac{aWU(F/400)}{d_{sc}^2 d_{sec}^2}$$
 - a = scatter fraction for 20 x 20 cm
 - F is maximum field area in cm²
 - NCRP 151 examples use $F=1600$ (conservative 40x40 cm field)
 - Effective F is smaller with IMRT
 - $F=225$ cm² w/ IMRT (15 x 15 cm)
 - $F = (1-\% \text{ IMRT}) \times 1600 + \% \text{ IMRT} \times 225$
 - Typically use $F=1600$ even if IMRT is used to add conservatism
 - Safety survey done w/o IMRT
 - IMRT seldom used at higher MV for dual energy machines
 - Primary beam adds to patient scatter at small scatter angles

- Scatter fraction as function of MV and scatter angle in NCRP 151 Table 5.4
- Scatter energy as function of MV and scatter angle in NCRP 151 Table B.6

Page 45

Use Factor (U) and Scatter

- Use Factor is typically taken as 1 for secondary calculations
 - Invariably true for leakage calculations
- Scatter is significant only for secondary barriers immediately adjacent to primary barriers
 - Scatter is negligible for all other orientations
 - NCRP 151: "However, if the [scatter] calculation is performed with the minimum angle of scatter from the patient to the point of calculation and a use factor of 1 is also used, the barrier thickness will be overestimated due to the conservatively higher scatter fraction from the smaller scattering angles"
- Sometimes appropriate to apply use factor to scatter
 - $U = 0.25$ appropriate if scatter angle $< 35^\circ$
 - i.e., secondary barrier immediately adjacent to primary barrier
 - $U=0.25$ best used only for retrofit (to avoid unnecessary modifications) or if there are severe space constraints
 - Otherwise $U = 1$

Page 46

Table 5: NCRP 151 Table B.4 Patient Scatter Fraction for 400 cm² Field

- Scatter fraction increases as angle decreases
- Scatter fraction vs MV may increase or decrease
 - Tends to increase with MV at small scatter angles
 - Decreases with increasing MV at large scatter angles

Linac MV	Angle (degrees)							
	10	20	30	45	60	90	135	150
4	1.04E-02	6.73E-03	2.77E-03	2.09E-03	1.24E-03	6.39E-04	4.50E-04	4.31E-04
6	1.04E-02	6.73E-03	2.77E-03	1.39E-03	8.24E-04	4.26E-04	3.00E-04	2.87E-04
10	1.66E-02	5.79E-03	3.18E-03	1.35E-03	7.46E-04	3.81E-04	3.02E-04	2.74E-04
15	1.51E-02	5.54E-03	2.77E-03	1.05E-03	5.45E-04	2.61E-04	1.91E-04	1.78E-04
18	1.42E-02	5.39E-03	2.53E-03	8.64E-04	4.24E-04	1.89E-04	1.24E-04	1.20E-04
20	1.52E-02	5.66E-03	2.59E-03	8.54E-04	4.19E-04	1.85E-04	1.23E-04	1.18E-04
24	1.73E-02	6.19E-03	2.71E-03	8.35E-04	3.91E-04	1.76E-04	1.21E-04	1.14E-04

Page 47

NCRP 151 Table B.6: Patient Scatter Energy

- Based on simulation by Taylor et al. (1999)

MV	Scatter Angle (degrees)							
	0	10	20	30	40	50	70	90
6	1.6	1.4	1.2	0.9	0.7	0.5	0.4	0.25
10	2.7	2.0	1.3	1.0	0.7	0.5	0.4	0.25
18	5.0	3.2	2.1	1.3	0.9	0.6	0.4	0.3
24	5.6	3.9	2.7	1.7	1.1	0.8	0.5	0.3

0.2 MV in NCRP 151, but 0.25 in Taylor et al.

Page 48

Scatter TVL Recommendations from NCRP 151

- Concrete TVL: NCRP 151 Table B.5a
 - Same values in 1976 NCRP 49 report
 - "Values ... are conservatively safe in nature" **Conservative**
- Lead scatter TVL: NCRP 151 Table B.5b (Nogueira and Biggs -- 2002)
 - Most accurate scatter TVLs in NCRP 151
 - Measurements and simulation in close agreement
 - For up to 10 MV and scatter angles $\geq 30^\circ$ **Accurate but limited**
- All other TVLs: NCRP 151 Figure A.1
 - Curves of equilibrium TVLs of shielding materials
 - NCRP 151 recommends using TVL corresponding to mean energy from NCRP 151 Table B6
 - Modifying the mean energy is recommended here **Rosetta Stone**

Table 6a. Concrete Scatter TVLs


Page 49

- Values directly from NCRP 151 Table B5.a
- Conservative at scatter angles less than 30°
 - Compared to lead and steel scatter TVLs

MV	Concrete Scatter TVL (mm)				
	Scatter Angle (degrees)				
	15	30	45	60	90
4	270	250	240	220	180
6	280	260	240	220	190
10	300	270	250	230	190
15	320	280	250	230	210
18	330	280	260	230	210
20	340	290	260	240	210
24	350	300	270	250	210

Broad Beam Equilibrium TVLs (NCRP 151 Figure A.1)

Page 50

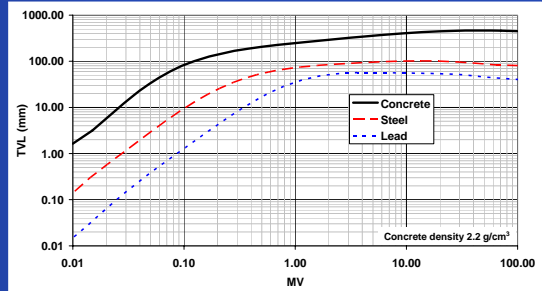

Lead Scatter TVL Recommendations Based on NCRP 151 [1 of 2]

Page 51

- NCRP 151 Table B.5b is the most reliable TVL data

MV	Lead scatter tenth-value layers (mm) vs. scatter angle											
	30		45		60		75		90			
	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe
4	33	37	24	31	18	25	13	19	9	13		
6	38	44	28	34	19	26	14	19	10	15		
10	43	45	31	36	21	27	15	19	12	16		

- First step: reconcile NCRP 151 Figure A.1 (broad beam transmission curves) with Table B.5b
 - TVLs in Table B.5b do not match NCRP 151 Figure A.1 using mean energy from NCRP 151 Table B.6
 - Equilibrium TVLs match if mean energy is multiplied by following adjustment factors

Broad Beam Energy Adjustment Factors					
MV	30	45	60	75	90
4	1.16	1.41	1.51	1.49	1.66
6	1.53	1.57	1.57	1.49	1.83
10	1.44	1.68	1.63	1.49	1.91

Lead Scatter TVL Recommendations Based on NCRP 151 [2 of 2]

Page 52

- Step 2: Select appropriate broad beam energy adjustments for other MVs

Broad Beam Energy Adjustment Factors						Adjusted Broad Beam Energy (MV)							
MV	20	30	45	60	75	90	MV	20	30	45	60	75	90
4	1.2	1.16	1.41	1.51	1.49	1.66	4	1.44	1.04	0.85	0.68	0.54	0.42
6	1.5	1.53	1.57	1.57	1.49	1.83	6	1.80	1.38	0.94	0.71	0.54	0.46
10	1.5	1.44	1.68	1.63	1.49	1.91	10	1.95	1.44	1.01	0.73	0.54	0.48
15	1.5	1.5	1.7	1.7	1.7	2.0	15	2.70	1.78	1.18	0.82	0.63	0.56
18	1.5	1.5	1.7	1.7	1.7	2.0	18	3.15	1.95	1.29	0.85	0.64	0.59
20	1.5	1.5	1.7	1.7	1.7	2.0	20	3.45	2.15	1.39	0.94	0.68	0.60
25	1.5	1.5	1.7	1.7	1.7	2.0	25	4.05	2.55	1.62	1.11	0.77	0.60

- Step 3: Read equilibrium lead TVLs From NCRP 151 Figure A.1 (conservatively use TVLe for TVL1)

Table 6b: Lead Scatter TVLs

MV	Lead Scatter tenth-value layers (mm)											
	20		30		45		60		75		90	
	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe	TVL1	TVLe
4	46	46	33	37	24	31	18	25	13	19	9	13
6	50	50	38	44	28	34	19	26	14	19	10	15
10	51	51	43	45	31	36	21	27	15	19	12	16
15	54	54	50	50	41	41	31	31	24	24	21	21
18	55	55	51	51	43	43	32	32	24	24	22	22
20	56	56	52	52	45	45	34	34	26	26	22	22
25	57	57	54	54	48	48	39	39	29	29	22	22

Table 6c. Steel Scatter TVL Recommendations Based on NCRP 151

Page 53


- Steel broad beam TVLs that correspond to the lead TVLs

MV	Recommended Steel Scatter TVL (mm)					
	Scatter Angle (degrees)					
	20	30	45	60	75	90
4	78	72	68	63	58	50
6	83	78	70	64	58	53
10	84	78	71	65	58	54
15	89	82	74	67	62	59
18	92	84	76	68	62	61
20	93	86	78	70	63	61
24	95	88	81	73	66	61

Patient Scatter Can Be Significant Adjacent to Primary Barrier

Page 54


- Both scatter fraction and scatter energy increase as scatter angle decreases
- Slant thickness compensates for the increased scatter
 - Required barrier thickness reduced by $\cos(\theta)$, where θ is slant angle
- Barrier thickness comparable to lateral barrier is typically adequate for same P/T



Primary Beam Remains Significant at Small Scatter Angles

Page 55

- Primary beam remains significant 1 ft beyond beam edge
 - 40x40 cm field rotated 45 degrees
 - Primary beam angle measured from target
 - Scatter angle measured from isocenter
- Conservatism in patient scatter shielding (i.e., $F=1600$) increases confidence edge of primary beam is adequately shielded
- Implications
 - Laminated primary barriers may need to extend more than 1 ft beyond the edge of beam
 - Recommend new primary barriers to be square, not tapered



Scatter Observations

Page 56

- Scatter is typically negligible for lateral barriers
- Must include scatter calculation for barrier next to primary
 - Particularly if slant factor is used when calculating photon leakage transmission
- General calculation procedure would include wall scatter also
 - Not addressed here since negligible for traditional secondary barriers
 - Vital to include for maze calculation for low energy linac

Maze Calculation

Page 57


- Specific scatter mechanisms included in maze calculation
 - Wall Scatter and Patient Scatter
 - Calculated at most stressing gantry orientation
 - Leakage scatter
- Direct leakage
 - Conventional secondary barrier calculation
 - If maze door lies beyond primary barrier, use primary barrier calculation instead
- High Energy accelerator mechanisms
 - Neutrons, capture gammas
 - Dominates the scatter mechanisms for high energy machines

Wall Scatter

Page 58

$$f H_S = f \frac{WU \alpha_0 A_0 \alpha_z A_z}{d_H^2 d_r^2 d_c^2}$$

- where
 - f = patient transmission (0.25)
 - α_0 = first reflection coefficient
 - NCRP 151 Table B.8a vs. MV
 - 75° angle of reflection typical
 - A_0 = beam area (m²) at wall
 - α_z = 2nd reflection coefficient
 - 0.5 MV at 75° in Table B.8a
 - A_z = Maze cross section (m²)
 - $w_m \times$ maze height



- Use factor adjustment
 - $U = 0.25$ applicable for above gantry orientation with highest dose rate
 - Total dose rate is 2.64 times the dose rate for this gantry angle

Beam Area at Wall

Page 59

- Beam area at wall (A_0) depends on distance from target
 - $A_0 = F (d_H / 1 \text{ m})^2$ (meters²)
 - F = Maximum field size at isocenter (1 m from target)
 - d_H = Distance from target to wall (also in meters)
- Traditional field size assumption
 - $F = 0.40 \text{ m} \times 0.40 \text{ m} = 0.16 \text{ m}^2$
 - NCRP 151 recommends traditional field size
- Alternative field size assumption with IMRT
 - With IMRT, maximum field typically 15 cm x 15 cm, or 0.0225 m²
 - Maximum field size 0.16 m² without IMRT
 - $F = (1\% \text{ IMRT}) \times 0.16 + \% \text{ IMRT} \times 0.0225$

Table 9. Reflection Coefficient for Concrete (NCRP 151 Tables B.8a and B.8b)

Page 60

MV	Angle of reflection measured from normal				
	0°	30°	45°	60°	75°
0.25	0.0320	0.0280	0.0250	0.0220	0.0130
0.5	0.0190	0.0170	0.0150	0.0130	0.0080
4	0.0067	0.0064	0.0058	0.0049	0.0031
6	0.0053	0.0052	0.0047	0.0040	0.0027
10	0.0043	0.0041	0.0038	0.0031	0.0021
18	0.0034	0.0034	0.0030	0.0025	0.0016
30	0.0030	0.0027	0.0026	0.0022	0.0015

MV	Angle of reflection measured from normal				
	0°	30°	45°	60°	75°
0.25	0.0360	0.0345	0.0310	0.0250	0.0180
0.5	0.0220	0.0225	0.0220	0.0200	0.0180
4	0.0076	0.0085	0.0090	0.0092	0.0095
6	0.0064	0.0071	0.0073	0.0077	0.0080
10	0.0051	0.0057	0.0058	0.0060	0.0060
18	0.0045	0.0046	0.0046	0.0043	0.0040
30	0.0048	0.0050	0.0049	0.0040	0.0030

- Reflection coefficient for steel or lead is 2x these values


Page 61

Patient Scatter

- Unshielded dose rate

$$H_{PS} = \frac{a W U (F/400) \alpha_1 A_1}{d_{sc}^2 d_{sec}^2 d_{zz}^2}$$

- where
 - α_1 is reflection coefficient
 - » NCRP 151 Table B.8b with 0.5 MV energy
 - » 0° angle of reflection
 - A_1 is maze wall area seen from the door
 - Other constants as before, e.g.,
 - » a = patient scatter fraction
 - See NCRP 151 Table B.4
 - » F = field size in cm²
 - » h = room height



- Use factor adjustment
 - U = 0.25 applicable for above gantry orientation with highest dose rate
 - Total dose rate is 2.64 times the dose rate for this gantry angle

Page 62

Table 5: NCRP 151 Table B.4 Patient Scatter Fraction for 400 cm² Field

- Scatter fraction increases as angle decreases
- Scatter fraction vs MV may increase or decrease
 - Tends to increase with MV at small scatter angles
 - Decreases with increasing MV at large scatter angles

Linac MV	Angle (degrees)							
	10	20	30	45	60	90	135	150
4	1.04E-02	6.73E-03	2.77E-03	2.09E-03	1.24E-03	6.39E-04	4.50E-04	4.31E-04
6	1.04E-02	6.73E-03	2.77E-03	1.39E-03	8.24E-04	4.26E-04	3.00E-04	2.87E-04
10	1.66E-02	5.79E-03	3.18E-03	1.35E-03	7.46E-04	3.81E-04	3.02E-04	2.74E-04
15	1.51E-02	5.54E-03	2.77E-03	1.05E-03	5.45E-04	2.61E-04	1.91E-04	1.78E-04
18	1.42E-02	5.39E-03	2.53E-03	8.64E-04	4.24E-04	1.89E-04	1.24E-04	1.20E-04
20	1.52E-02	5.66E-03	2.59E-03	8.54E-04	4.13E-04	1.85E-04	1.23E-04	1.18E-04
24	1.73E-02	6.19E-03	2.71E-03	8.35E-04	3.91E-04	1.76E-04	1.21E-04	1.14E-04

Repeat of Table 5 Used for Secondary Barrier Calculations


Page 63

Leakage Scatter

- Unshielded dose rate

$$H_{LS} = \frac{10^{-3} W_L U \alpha_1 A_1}{d_{sec}^2 d_{zz}^2}$$

- where
 - 10⁻³ = head-leakage radiation ratio
 - α_1 is reflection coefficient
 - » NCRP 151 Table B.8b with MV = 1.4 at 6 MV, 1.5 at 10 MV
 - » 0° angle of reflection
 - A_1 is maze wall area seen from door
 - d_{sec} measured from isocenter
 - » Isocenter is average target location



- Use factor adjustment
 - NCRP 151 recommends same adjustment as patient and wall scatter
 - U = 1 with no adjustment is assumed in the example calculations here
 - » with d_{sec} measured from isocenter


Page 64

Direct Leakage

- Unshielded dose rate

$$H_{LR} = \frac{10^{-3} W_L U B}{d_L^2}$$

- Same as standard secondary photon leakage calculation
 - B is leakage transmission through wall
- Use factor adjustment
 - NCRP 151 recommends the same adjustment as patient and wall scatter
 - U = 1 with no adjustment is assumed in the example calculations here




Page 65

Tenth-Value Layers for Maze Calculation

- Patient and wall scatter TVLs based on 0.2 MV broadbeam transmission
 - TVL read from NCRP 151 Figure A.1
 - Low energy since two bounces
- Leakage scatter TVLs based on 0.3 MV broadbeam transmission
 - 0.3 MV average energy cited in McGinley p. 49
 - » Single bounce vs. two bounces for patient & wall scatter
 - TVL read from NCRP 151 Figure A.1
- Leakage TVL for direct leakage
 - Note that door may not shield direct leakage for short maze

Page 66

Broad Beam Equilibrium TVLs (NCRP 151 Figure A.1)

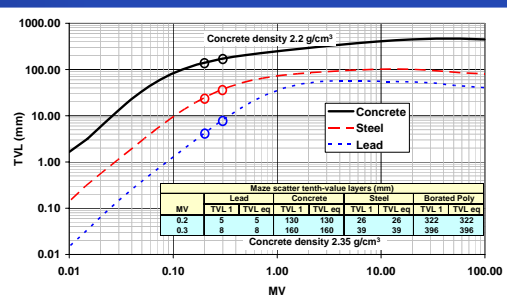

MV	Lead			Concrete		Steel		Borated Poly	
	TVL-1	TVL-2	TVL-3	TVL-1	TVL-2	TVL-1	TVL-2	TVL-1	TVL-2
0.2	5	5	130	130	26	26	322	322	
0.3	8	8	160	160	39	39	396	396	

Concrete density 2.35 g/cm³

Maze Calculations for High Energy Accelerators


Page 67

- Neutrons and capture gammas dominate the shielded dose
- Direct leakage may also be significant
 - Particularly with thin maze wall
- Scatter mechanisms continue to apply
 - But are invariably negligible for MV > 10

Maze Neutron and Capture Gammas: NCRP 151

Page 68

- First step: Calculate neutron fluence at point A
- Second step: Calculate unshielded capture gamma dose rate at door
 - Uses neutron fluence at point A
- Third step: Calculate unshielded neutron dose-equivalent rate at door
 - Uses neutron fluence at point A
- Fourth step: Calculate attenuation of maze neutrons & capture gammas by the door



Neutron Fluence Calculation

Page 69

- Neutrons / m² / Gy workload

$$\phi_A = \frac{\beta Q_n}{4\pi d_1^2} + \frac{5.4\beta Q_n}{2\pi S_r} + \frac{1.3 Q_n}{2\pi S_r}$$

- 1st term: Direct neutrons
- 2nd term: Scattered neutrons
- 3rd Term: Thermal neutrons

where

- β = head shielding transmission factor = 1.0 for lead, 0.85 for tungsten
 - d_1 = Distance from isocenter to point A
 - Q_n = Neutron source strength (Table 10)
 - S_r = Treatment room surface area (m²)
- $$S_r = 2(d_L d_w + h d_L + h d_w) \quad \text{where } h \text{ is vault height}$$




Table 10: NCRP 151 Table B.9 Total Neutron Source Strength (Q_n)

Page 70

Vendor	MV	Q _n N/Gy
Varian	10	6.0E+10
	15	7.6E+11
	18	9.6E+11
	20	9.6E+11
Siemens	24	7.7E+11
	10	8.0E+10
	15	2.0E+11
	18	8.8E+11
Elekta / Philips	20	9.2E+11
	24	1.5E+12
	10	1.4E+11
	15	3.2E+11
GE	18	6.9E+11
	20	9.6E+11
	24	1.4E+12
	12	2.4E+11
	15	4.7E+11
	18	1.5E+12
	25	2.4E+12

Maze Capture Gamma Unshielded Dose Rate Calculation

Page 71

- Capture gamma dose at door per workload at isocenter (Sv/Gy)

$$h_\phi = K \phi_A 10^{(-d_2 / TVD)}$$


where

- K = ratio of capture gamma dose at point A to neutron fluence = 6.9×10^{-16} m² Sv / neutron
- d_2 = distance from point A to door
- TVD = tenth-value distance (m) = 5.4 for 18-24 MV, 3.9 for 15 MV

- Weekly capture gamma dose rate at door

$$H_{cg} = W_{Ln} h_\phi$$

– W_{Ln} is neutron leakage workload



Maze Neutron Unshielded Dose Rate Calculation

Page 72

- Maze neutron dose-equivalent at door per neutron leakage workload at isocenter (Sv/Gy)


$$H_{n,D} = 2.4 \times 10^{-15} \phi_A \left[\frac{S_0}{S} \right]^{1/2} \left[1.64 \times 10^{(-d_2 / 1.9)} + 10^{(-d_2 / TVD)} \right]$$

where

- S_0 / S = ratio of inner maze entrance cross-section area ($S_0 = d_0 h$) to maze cross-section area ($S = d_M h$)
- d_2 = distance from point A to door
- TVD = tenth-value dist. = $2.06 S^{1/2}$

- Weekly neutron dose-equivalent at door

$$H_n = W_{Ln} H_{n,D}$$



Maze Door Neutron Shielding TVL

Page 73

- 45 mm TVL_n for borated polyethylene
 - “maze door shielding, a conservatively safe recommendation is that a TVL of 4.5 cm be used in calculating the borated polyethylene (BPE) thickness requirement” [NCRP 151 p. 46]
- 161 TVL_n for concrete wall adjacent to door
 - “the average neutron energy at the maze entrance is reported to be ~100 keV” [also NCRP 151 p. 46]
 - NCRP 79 TVL_n for concrete with 0.1 MV neutron energy
 - » TVL_n = 155 + 56 * 0.1 = 161 mm

Maze Capture Gamma TVL

Page 74

- NCRP 151
 - “for very short mazes ... a lead TVL of 6.1 cm may be required”
 - “mazes longer than 5 m ...TVL of only about 0.6 cm lead”
- Reading between the lines
 - Use 61 mm TVL for lead (NCRP 79) regardless of maze length
 - “The average energy of neutron capture gamma rays is 3.6 MeV”
 - » Assumed to apply to long mazes ($d_2 > 5$ m)
 - » Use NCRP 151 Figure A.1 TVLs at 3.6 MV for concrete / steel
 - “can range as high as 10 MeV” for very short mazes
 - » Short maze assumed to be $d_2 \leq 2.5$ m
 - » Use primary 10 MV TVLs (except 61 mm for lead vs. 57 mm 10 MV TVL)
 - “conservatively safe if one assumes that all neutron captures result in 7.2 MeV gamma rays” for direct-shielded doors
 - » Assumed to be conservatively safe for $2.5 \text{ m} < d_2 \leq 5 \text{ m}$ maze also
 - » Interpolate NCRP 151 Table B.2 TVLs at 7.2 MV for concrete / steel

Table 11. Maze Neutron and Capture Gamma TVL Summary

Page 75

Maze Neutron tenth-value layers (mm)								
MV	Lead		Concrete		Steel		Borated Poly	
	TVL 1	TVL eq	TVL 1	TVL eq	TVL 1	TVL eq	TVL 1	TVL eq
0.1	N/A	N/A	161	161	N/A	N/A	45	45

Capture Gamma tenth-value layers (mm)									
MV	Lead		Concrete		Steel		Borated Poly		Distance Pt. A to Door
	TVL 1	TVL eq	TVL 1	TVL eq	TVL 1	TVL eq	TVL 1	TVL eq	
3.6	61	61	330	330	95	95	817	817	$d_2 > 5 \text{ m}$
7.2	61	61	390	350	103	103	965	866	$2.5 \text{ m} < d_2 < 5 \text{ m}$
10	61	61	410	370	110	110	1015	916	$d_2 < 2.5 \text{ m}$

Direct-Shielded Door

Page 76

- Neutron Door is simply a secondary barrier
 - Typically more layers and different materials than a wall
 - » Lead to attenuate leakage photons
 - » Borated polyethylene to attenuate leakage neutrons
 - Typically sandwiched between layers of lead
 - » Steel covers
- Specialized shielding procedure adjacent to door
 - Compensates for relatively small slant thickness in this location
 - Vault entry toward isocenter similar to maze
 - Vault entry away from isocenter is secondary barrier
 - » But with specialized geometry

Factor of 2 to 3 Margin Recommended for Direct Shielded Doors


Page 77

- NCRP 151 recommends considering capture gammas for direct-shielded doors (Section 2.4.5.2)
 - Recommendation is to add 1 HVL to leakage calculation for door only, but not for walls
 - » Rationale: Concrete in wall is more effective for capture gammas than material in door
 - Equivalently, factor of 2 margin on shielded dose rate relative P/T
- Dose rate from HVAC duct above door comparable to dose rate through door
 - Additional reason to provide margin on door calculation

Direct-Shielded Door: Far Side of Entrance

Page 78


- Extra material added to corner
 - Lead to entrance wall
 - Borated polyethylene or concrete beyond wall
- Uses standard secondary barrier calculation
- Goal: provide same protection as wall or door for path through corner

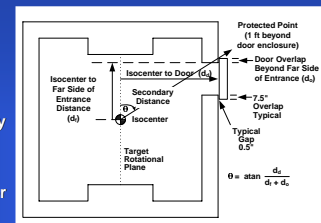

Direct-Shielded Door: Near Side of Entrance Wall Scatter

Page 79


- Geometry similar to short maze
 - Maze calculation is reasonable to use
- Requires less material than far side of entrance
 - Lower unshielded dose rate
 - Lower energy
- Wall scatter determines shielding for < 10 MV
 - Not significant if high energy

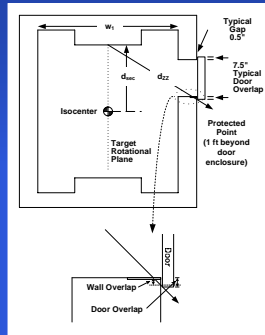

Direct-Shielded Door: Near Side of Entrance Neutrons / Capture Gammas

Page 80

- Geometry similar to short maze
 - Maze calculation is reasonable to use
- Requires less material than far side of entrance
 - Lower unshielded dose rate
 - Lower energy



Shielding for Heating, Ventilation, and Air Conditioning (HVAC) Ducts

Page 81

- HVAC penetration is located at ceiling level in the vault
 - For vaults with maze, typically located immediately above door
 - For direct-shielded doors, located in a lateral wall parallel to the plane of gantry rotation as far away from isocenter as possible
- Ducts shielded with material similar to the door at entrance
- For direct-shielded door, thickness 1/2 to 1/3 of the door
 - Path through material is at a very oblique angle due to penetration location with slant factor between 2 and 3
 - Factor of at least 5 reduction in dose at head level (the protected location) vs. at the HVAC duct opening
- Even less material is required for maze duct
 - NCRP 151 example is 3/8" lead plus 1" BPE extending 4 ft

Primary and Secondary Barrier Examples

Page 82

1. Basic primary barrier photon shielded dose rate
2. Minimum width of primary barrier
3. Secondary barrier photon leakage
4. Secondary barrier photon leakage with IMRT
5. Secondary barrier photon & neutron leakage with IMRT
6. Secondary barrier photon & neutron leakage plus patient scatter with IMRT
- 7,8. Secondary barrier calculation including slant factor

Maze and Direct Shielded Door Calculation Examples


Page 83

9. Maze with secondary leakage through door, 6 MV
10. Maze with secondary leakage through door, 18 MV
11. Direct shielded door in secondary barrier

Example 1: 18 MV Primary Concrete Barrier

Page 84

1. Establish P/T for protected location A: $P/T = 0.1 \text{ mSv/wk}$ ($P = 0.1 \text{ mSv/wk}$, $T = 1$)
2. Measure distance from target to protected location (22 ft from target)
3. Measure (or read from annotations) the barrier material thickness (7 ft)
4. Determine TVLs based on MV (18) and material type (concrete)
5. Calculate unshielded dose rate, transmission, and shielded dose rate (add or increase material until shielded dose rate < P/T)

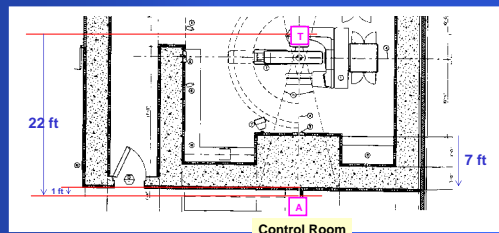

Page 85

Example 1: P/T Calculation for Primary Barrier

Line	Parameter	Units	Value	Calculation
a	Design Dose Limit (P)	mSv/wk	0.1	
b	Occupancy Factor (T)		1	
c	Weekly Protect P/T Limit	mSv/wk	0.100	a / b
d	Dose Limit Per Hour	mSv/hr	0.02	
e	Dose per Patient Treatment	Gy/pt	3	Default value
f	Patients per Day	pt/day	30	Default value
g	Workload (W) per Week	Gy/wk	450	5 * e * f
h	Max patient / hr	patient	6	
i	Max Workload / Hour (W _h)	Gy/hr	3.6	h * e / 5
j	Hourly Protect P/T Limit	mSv/wk	2.500	0.02 * g / i
k	P/T	mSv/wk	0.100	min{c, j}

Weekly P/T Limit

Hourly limit converted to equivalent weekly P/T limit

P/T = 0.1 mSv/wk

Cells with inputs are shaded green

- Hourly protection limit does not impact P/T for high occupancy location
- Hourly protection limit may impact P/T for low occupancy locations in uncontrolled areas

Page 86

Example 1: Shielded Photon Dose Calculation

Line	Parameter	Units	Value	Calculation
a	Machine X-ray Energy	MV	18	
b	Workload (W)	Gy/Wk	450	
c	Use Factor		0.25	
d	Target to Protected Point Distance	ft	22	
e		m	6.71	d * 0.3048
f	Unshielded Dose	mSv/wk	2.50E+03	1000 * b * c / e ²
g	Total Photon Transmission		(1.22E-05)	see below
h	Shielded Photon Dose	mSv/wk	0.030	f * g

0.030 mSv is less than P/T = 0.1 mSv/wk

Key inputs to the calculation

Barrier	Material Thickness		Material	X-Ray Primary		Photon Trans.
	inches	mm		TVL1 (mm)	TVLc (mm)	
Inside Layer	84	2134	Concrete	450	430	1.22E-05
Layer #2						1.00E+00
Outside Layer						1.00E+00
				18 MV	Total:	1.22E-05

Photon transmission through concrete = $0.1 \cdot 10^{-4} \cdot (2134 - 450 / 430) = 1.22E-5$

TVLs are function of MV and Concrete

Page 87

Example 2a. Traditional Primary Barrier Minimum Width

Line	Parameter	Units	Value	Calculation
a	Target to Narrow Point	ft	18	
b	Target to Narrow Point	m	5.49	a * 0.3048
c	Effective field size (corners)	cm	35	
d	Max Field Diameter	m	2.72	b * sqrt(2) * c / 100
e	Max Field Diameter	ft	8.9	d / 0.3048
f	Minimum Barrier Width	ft	10.9	e + 2 ft
g	Recommended Width	ft	11	

Page 88

Example 2b. Recommended Primary Barrier Minimum Width in NCRP 151

- NCRP 151 recommends calculating barrier width at top of primary barrier
- Requires ~ 1 ft increase in primary barrier width compared to traditional calculation in Example 2a.
- Appropriate for new construction
- Perhaps inappropriate for retrofit to existing vault
 - Especially for ceiling or exterior wall with no occupancy above ceiling

Line	Parameter	Units	Value	Calculation
a	Distance from target to narrow point	ft	18	
b	Distance from target to narrow point	m	5.49	a * 0.3048
c	Effective field size (corners)	cm	35	
d	Distance from isocenter to ceiling	ft	7	
e		m	2.13	d * 0.3048
f	Target to top of narrow point	m	5.97	sqrt(e ² + (b-1) ²) + 1
g	Maximum Field Diameter	m	2.95	f * sqrt(2) * c / 100
h		ft	9.7	g / 0.3048
i	Minimum Barrier Width	ft	11.7	h + 2 ft
j	Recommended Width	ft	12	

Page 89

Example 3: 6 MV Secondary Barrier Leakage (Existing Construction)

- Establish P/T for protected location:
 - Uncontrolled location P = 0.02 mSv/wk
 - Low occupancy location (closet)
 - T = 0.05
 - P/T = 0.400
- Measure distance from isocenter to protected location
 - 14 ft from isocenter to 1 ft beyond wall
- Measure (or read from annotations) the barrier material thickness (26 in)
- Low usage facility in small town justifies lower than typical workload
 - 25 patients per day at 3 Gy/treatment
 - Yields 375 Gy/wk vs. 450 Gy/wk typical assumption
 - IMRT not available at facility

Calculate unshielded dose rate, transmission, & shielded dose rate (add or increase material until shielded dose rate < P/T)

Page 90

Example 3: Leakage Calculation (Existing Construction)

Line	Parameter	Units	Value	Calculation
a	Workload / Treatment	Gy/pt	3	Default value
b	Patients per Day	pt/day	25	Anticipated
c	Workload (W)	Gy/wk	375	5 * a * b
d	Use Factor	Ratio	1	
e	Leakage Fraction	Ratio	1.0E-03	
f	Isocenter to Protected Point Distance	ft	13.5	
g		m	4.11	f * 0.3048
h	Unshielded Dose	mSv/wk	2.21E+01	1000 * c * d * e / g ²
i	Transmission		7.86E-03	see below
j	Shielded Dose	mSv/wk	0.174	h * i

0.174 mSv is less than P/T = 0.400 mSv/wk

Barrier	Material Thickness		Material	X-Ray Leakage		Photon Trans.
	inches	mm		TVL1 (mm)	TVLc (mm)	
Inside Layer	26	660	Concrete	340	290	7.86E-03
Layer #2						1.00E+00
Layer #3						1.00E+00
Layer #4						1.00E+00
Outside Layer						1.00E+00
				6 MV	Total:	7.86E-03

Photon transmission through concrete = $0.1 \cdot 10^{-4} \cdot (660 - 340 / 290) = 7.86E-3$

Page 91

Example 4: 6 MV Additional Shielding with IMRT

- Establish P/T for protected location
 - Dressing room uncontrolled with partial occupancy (T=0.2)
 - P/T = 0.10 mSv/wk
- Measure distance from target to protected location
 - 14 ft from target to 1 ft beyond wall
- Measure (or read from annotations) the barrier material thickness (26 in)
- IMRT factor 2
 - 50% IMRT workload with IMRT ratio 3
- Facility expects increased usage
 - Default 30 patients per day assumed vs. 25
- Add additional lead to barrier until shielded dose rate is less than P/T
 - Can be either inside or outside wall for secondary barrier

Page 92

Example 4: Leakage Calculation with IMRT

Line	Parameter	Units	Value	Calculation
a	Workload / Treatment	Gy/pt	3	Default value
b	Patients per Day	pt/day	30	Default value
c	Workload (W)	Gy/wk	450	a * b
d	Use Factor	Ratio	1	
e	Leakage Fraction	Ratio	1.0E-03	
f	IMRT Factor		2	
g	Isocenter to Protected Point Distance	ft	13.5	
h		m	4.1	g * 0.3048
i	Unshielded Dose	mSv/wk	5.32E+01	1000*c*d*e/fh^2
j	Transmission		1.29E-03	see below
k	Shielded Dose	mSv/wk	0.069	i * j

0.069 mSv is less than P/T = 0.10 mSv/wk

Barrier	Material Thickness		Material	X-Ray Leakage		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	1.5	38	Lead	57	57	2.15E-01
Layer #2	26	660	Concrete	340	290	6.02E-03
Outside Layer						1.00E+00
				6 MV	Total:	1.29E-03

Photon transmission through lead = $10^{-(38/57)} = 0.215$ $340^{-(1-38/57)} = 113$
 Photon transmission through concrete = $10^{-(113/340)} = 10^{-(660-113)/290} = 6.0E-3$
 Total transmission = transmission through lead x transmission through concrete

Page 93

Example 5: 15 MV Secondary Barrier Photon & Neutron Leakage (Additional Shielding)

- Establish P/T (0.10 mSv/wk)
- Isocenter to protected location distance
 - 14 ft from target to 1 ft beyond wall
- Existing barrier 26 in concrete
- IMRT factor 2 for photons, 1 neutrons
 - Most IMRT is performed at 6 MV energy
- Default 450 Gy/wk workload
- Calculate unshielded dose rate, transmission, and shielded dose rate
- Add additional lead to barrier until shielded dose rate is less than P/T
 - 2" lead added to inside of barrier
 - Can be outside if space inadequate inside
 - No photoneutron generation for lead in secondary barriers

Page 94

Example 5: 15 MV Secondary Barrier Photon and Neutron Leakage Calculation

Line	Parameter	Units	Photon Leakage	Neutron Leakage	Calculation
a	Workload / Treatment	Gy/pt	3	3	Default value
b	Patients per Day	pt/day	30	30	Default value
c	Workload (W)	Gy/wk	450	450	5 * a * b
d	Use Factor	Ratio	1	1	
e	Leakage Fraction	Ratio	1.0E-03	7.0E-04	15 MV values
f	IMRT Factor		2	1	
g	Isocenter to Protected Point Distance	ft	13.5	13.5	
h		m	4.1	4.1	g * 0.3048
i	Unshielded Dose	mSv/wk	5.32E+01	1.86E+01	1000*c*d*e/fh^2
j	Transmission		1.31E-03	7.42E-04	see below
k	Shielded Dose	mSv/wk	0.070	0.014	i * j
L	Total Shielded Dose	mSv/wk	0.083		Sum row k

0.083 mSv is less than P/T = 0.100 mSv/wk

Barrier	Material Thickness		Material	X-Ray Leakage		Photon Trans.	Neutron TVL (mm)	Neutron Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)			
Inside Layer	2	51	Lead	57	57	1.29E-01	N/A	1.00E+00
Layer #2	26	660	Concrete	360	330	1.02E-02	211	7.42E-04
Outside Layer						1.00E+00		1.00E+00
				15 MV	Total:	1.31E-03	Total:	7.42E-04

Neutron leakage calculation similar in form to photon leakage calculation, except using different leakage fraction and TVLs

Page 95

Example 6: 15 MV Secondary Barrier Including Leakage and Scatter

- Follow same first steps of Example 5 leakage calculation (establish P/T, distances, material thickness & type, IMRT factors)
- Determine scatter fraction per 400 cm² by interpolating scatter fraction as a function of MV and scatter angle (Table 6)
- Calculate effective field size
- Determine scatter fraction by adjusting scatter per 400 cm² with effective field size
- Calculate unshielded dose rate
- Interpolate TVL using Table 7 as a function of machine MV, material type and scatter angle
- Calculate transmission and shielded dose rate (add or increase material until shielded dose rate < P/T)

Page 96

Example 6: Secondary Barrier Scatter Fraction Calculation

Line	Parameter	Units	Value	Calculation
a	Design Dose Limit (P)	mSv/wk	0.02	
b	Occupancy Factor (T)		0.2	
c	P/T	mSv/wk	0.100	a / b
d	Machine X-ray Energy	MV	15	
e	Vendor	Varian		

Line	Parameter	Units	Value		Calculation
			w/o IMRT	with IMRT	
a	Max Field Size	cm	40	15	
b	Fraction of Workload		50%	50%	
c	Effective Field Area	cm ²	912.5		b ₁ * a ₁ ² + b ₂ * a ₂ ²
d	Effective Field Size	cm	30.2		sqrt (c)
e	Scatter Angle	deg	90		
f	Machine X-ray Energy	MV	15		
g	Scatter / 400 cm ²		2.61E-04		Function of e & f
h	Scatter Fraction		0.00060		g * c / 400

Illustrates using effective field size with 15x15 cm IMRT field

Page 97

Example 6: Secondary Barrier Shielded Dose Rate Calculation Including Leakage & Scatter

Line	Parameter	Units	Leakage	Scatter	Leakage	Calculation
a	Workload / Treatment	Gy/pt	3	3	3	NCRP 151 Default
b	Patients per Day	pt/day	30	30	30	NCRP 151 Default
c	Workload (W)	Gy/wk	450	450	450	a * b
d	Use Factor	Ratio	1	1	1	
e	Fraction	Ratio	1.0E-03	6.0E-04	7.0E-04	15 MV values
f	IMRT Factor		2	1	1	
g	Isocenter to Protected Point Distance	ft	13.5	13.5	13.5	
h		m	4.1	4.1	4.1	g * 0.3048
i	Unshielded Dose	mSv/wk	5.32E+01	1.58E+01	1.86E+01	1000*c*d*e*f/h^2
j	Transmission		4.59E-04	5.04E-08	7.42E-04	see below
k	Shielded Dose	mSv/wk	0.024	0.000	0.14	i * j
L	Total Shielded Dose	mSv/wk	0.038			Sum row k

0.038 mSv is less than P/T = 0.100 mSv/wk

Barrier	Material Thickness		Photon Leakage			Scatter			Neutron		
	Inches	mm	TVL1(mm)	TVL2(mm)	Trans.	TVL1(mm)	TVL2(mm)	Trans.	TVL (mm)	Trans.	
Inside Layer	3	76	Lead	57	57	4.60E-02	21	21	2.35E-04	N/A	1.00E+00
Layer #2	26	660	Concrete	N/A	330	9.97E-03	180	180	2.14E-04	211	7.42E-04
Layer #3						1.00E+00			1.00E+00		1.00E+00
Outside Layer						1.00E+00			1.00E+00		1.00E+00
				15 MV	Total:	4.59E-04	Total:	5.04E-08	Total:	7.42E-04	

Scatter is typically negligible for lateral secondary barrier, but neutron leakage can be significant

Page 98

Example 7: Secondary Barrier Adjacent to Primary

- Establish P/T for protected location C: P/T = 0.1 mSv/wk
- Distance from isocenter to protected location: 22 ft
- Secondary barrier 3 ft concrete, slant thickness 3 ft / cos(25°)
- Calculate scatter fraction based on scatter angle and average field size
- Calculate shielded dose rate comprised of photon leakage, neutron leakage and scatter using slant thickness for transmission (add material or increase thickness until < P/T)

Page 99

Example 7: Secondary Barrier Scatter Fraction Calculation

Line	Parameter	Units	Value	Calculation
a	Design Dose Limit (P)	mSv/wk	0.1	
b	Occupancy Factor (T)		1	
c	P/T	mSv/wk	0.100	a / b
d	Machine X-ray Energy	MV	18	
e	Vendor		Varian	

Line	Parameter	Units	Value		Calculation
			w/o IMRT	with IMRT	
a	Max Field Size	cm	40	40	
b	Fraction of Workload		50%	50%	
c	Effective Field Area	cm^2	1600.0		b ₁ *a ₁ ² + b ₂ *a ₂ ²
d	Effective Field Size	cm	40.0		sqrt (c)
e	Scatter Angle	deg	25		
f	Machine X-ray Energy	MV	18		
g	Scatter / 400 cm^2		3.89E-03		Function of e & f
h	Scatter Fraction		0.01477		g * c / 400

Illustrates using conservative F = 1600 cm² field area assumption

Page 100

Example 7: Secondary Barrier Calculation Including Leakage, Scatter, & Slant Thickness

Line	Parameter	Units	Photon Leakage	Photon Scatter	Neutron Leakage	Calculation
a	Workload / Treatment	Gy/pt	3	3	3	NCRP 151 default
b	Patients per Day	pt/day	30	30	30	NCRP 151 default
c	Workload (W)	Gy/wk	450	450	450	a * b
d	Use Factor	Ratio	1	1	1	adjacent to pri barrier
e	Fraction	Ratio	1.0E-03	1.5E-02	1.5E-03	Varian at 18 MV
f	IMRT Factor		2	1	1	
g	Isocenter to Protected Point Distance	ft	21.0	21.0	21.0	
h		m	6.4	6.4	6.4	g * 0.3048
i	Unshielded Dose	mSv/wk	2.20E+01	1.62E+02	1.65E+01	1000*c*d*e*f/h^2
j	Transmission		3.72E-04	4.66E-04	1.65E-05	see below
k	Shielded Dose	mSv/wk	0.008	0.076	0.000	i * j
L	Total Shielded Dose	mSv/wk	0.084			Sum row k

0.084 mSv is less than P/T = 0.100 mSv/wk

Barrier	Material Thickness		Photon Leakage			Scatter			Neutron		
	Inches	mm	Material	TVL1 (mm)	TVL2 (mm)	Trans.	TVL1 (mm)	TVL2 (mm)	Trans.	TVL (mm)	Trans.
Inside Layer	1	25	Lead	57	57	3.22E-01	53	53	2.96E-01	N/A	1.00E+00
Layer #2	36	1009	Concrete	360	340	1.15E-03	360	360	1.58E-03	211	1.65E-05
Layer #3						1.00E+00			1.00E+00		1.00E+00
Layer #4						1.00E+00			1.00E+00		1.00E+00
Outside Layer						1.00E+00			1.00E+00		1.00E+00
Slant Angle (degrees):			25	18 MV	Total:	3.72E-04	Total:	4.66E-04	Total:	1.65E-05	

Page 101

Example 8: Scatter Adjacent to Primary Barrier

- Establish P/T for location D: P = 0.02 mSv, T = 0.2, P/T = 0.10 mSv/wk
- Distance from isocenter to protected location: 14.5 ft
- Secondary barrier 2" lead and 30" concrete, 15° slant angle
- Determine scatter fraction per 400 cm² by interpolating scatter fraction table as a function of MV (18) and scatter angle (30°)
- Calculate effective field size, scatter fraction
- Calculate shielded dose rate comprised of photon leakage, neutron leakage and scatter using slant thickness for transmission

Page 102

Example 8: Secondary Barrier Scatter Fraction Calculation

Line	Parameter	Units	Value	Calculation
a	Design Dose Limit (P)	mSv/wk	0.02	
b	Occupancy Factor (T)		0.2	
c	P/T	mSv/wk	0.100	a / b
d	Machine X-ray Energy	MV	18	
e	Vendor		Varian	

Line	Parameter	Units	Value		Calculation
			w/o IMRT	with IMRT	
a	Max Field Size	cm	40	40	
b	Fraction of Workload		50%	50%	
c	Effective Field Area	cm^2	1600.0		b ₁ *a ₁ ² + b ₂ *a ₂ ²
d	Effective Field Size	cm	40.0		sqrt (c)
e	Scatter Angle	deg	30		
f	Machine X-ray Energy	MV	18		
g	Scatter / 400 cm^2		2.53E-03		Function of e & f
h	Scatter Fraction		0.01012		g * c / 400

Example 8: Secondary Barrier Shielded Dose Rate Calculation Including Leakage & Scatter

Page 103

Line	Parameter	Units	Photon Leakage	Photon Scatter	Neutron Leakage	Calculation
a	Workload / Treatment	Gy/pt	3	3	3	NCRP 151 default
b	Patients per Day	pt/day	30	30	30	NCRP 151 default
c	Workload (W)	Gy/wk	450	450	450	5 * a * b
d	Use Factor	Ratio	1	0.25	1	adjacent to pri barrier
e	Fraction	Ratio	1.0E-03	1.0E-02	1.5E-03	Varian at 18 MV
f	IMRT Factor		2	1	1	
g	Isocenter to Protected Point Distance	ft	14.5	14.5	14.5	
h		m	4.4	4.4	4.4	g * 0.3048
i	Unshielded Dose	mSv/wk	4.61E+01	5.83E+01	3.46E+01	1000*c*d*e ² /h*2
j	Transmission		5.78E-04	3.19E-04	1.82E-04	see below
k	Shielded Dose	mSv/wk	0.027	0.019	0.006	i * j
L	Total Shielded Dose	mSv/wk				Sum row k


0.052 mSv is less than P/T = 0.10 mSv/wk

Barrier	Material Thickness (inches)	Material Thickness (mm)	Material	Photon Leakage TVL1 (mm)	Photon Leakage TVLc (mm)	Trans.	Scatter TVL1 (mm)	Scatter TVLc (mm)	Trans.	Neutron TVL (mm)	Trans.
Inside Layer	2	53	Lead	57	57	1.19E-01	51	51	3.31E-02	N/A	1.00E+00
Layer #2						1.00E+00			1.00E+00		1.00E+00
Layer #3						1.00E+00			1.00E+00		1.00E+00
Outside Layer	30	789	Concrete	360	340	4.83E-03	320	320	3.43E-03	211	1.82E-04
Slant Angle (degrees):	15			18 MV	Total:	5.78E-04	Total:	3.19E-04	Total:	1.82E-04	

Example 9: Conventional Maze, 6 MV

Page 104


- Conventional maze similar to NCRP 151 examples
 - Axis of rotation is parallel to maze; maze extends full length of vault
- Machine energy is 6 MV
 - All scatter mechanisms must be calculated
 - Direct leakage must also be calculated
 - With door also contributing to attenuation of direct leakage
 - Neutron & capture gamma calculation is not needed
 - < 10 MV

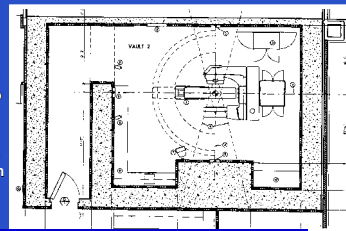

Door: 0.25" lead, hard wood covers

Example 9a: Patient Scatter

Page 105

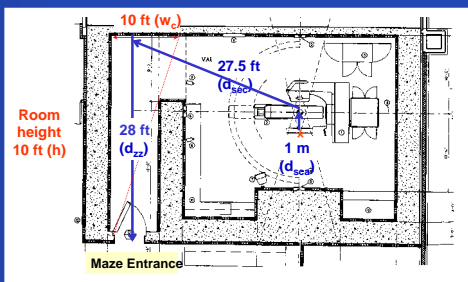

Example 9: P/T and Average Field Size Calculation

Page 106

- Protected location is in a controlled area (P= 0.1 msv/wk)
 - NCRP 151 occupancy T=1/8 for extremely low traffic location
 - Higher occupancy appropriate if close proximity to control area
 - e.g., T=0.5 or T=1 (T=1 is assumed in example)
 - Maximum shielded dose rate (P/T) is 0.1 mSv/wk for T=1
- NCRP 151 examples uses 40 x 40 cm² field area for scatter
 - Weighted average field area with / without IMRT also valid
 - e.g., especially useful for existing vault door calculations
 - Caution: Safety survey often performed without IMRT

Line	Parameter	Units	Value		Calculation
			w/o IMRT	with IMRT	
a	Max Field Size	cm	40	40	
b	Fraction of Workload		50%	50%	
c	Effective Field Area	cm ²	1600		b ₁ * a ₁ ² + b ₂ * a ₂ ²
d	Effective Field Size	cm	40.0		sqrt (c)


Example 9a: Patient Scatter Unshielded Dose Rate Calculation

Page 107

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	6	
b	W	Workload	Gy/wk	450	
c	d _{scs}	Distance from target to isocenter	m	1.00	
d	d _{sc}	Distance from isocenter to wall at maze end	ft	27.5	measured
e			m	8.38	d * 0.3048
f	d _w	Distance from wall at maze end to door	ft	28	measured
g			m	8.53	f * 0.3048
h	w ₁	Wall width seen from door	ft	10	measured
i			m	3.05	h * 0.3048
j	h	Room height	ft	10	measured
k			m	3.05	j * 0.3048
L	A ₁	Scatter area	m ²	9.3	i * k
m	a	Patient scatter fraction (400 cm ² field)		1.39E-03	See Table 5 (45°) Function of MV
n	α ₁	Reflection Coefficient		2.20E-02	Table 8a, 0.5 MV, 45°
o	F	Average field area	cm ²	1600	See above
p	U	Use Factor		0.25	Orientation with highest dose rate
q	H _{PS}	Patient scatter unshielded dose rate	mSv/wk	2.50E-02	1000 * m * p * q / (400) * L / (c ² * e ² * g ²)

Example 9b: Maze with Secondary Leakage Through Door — Wall Scatter

Page 108

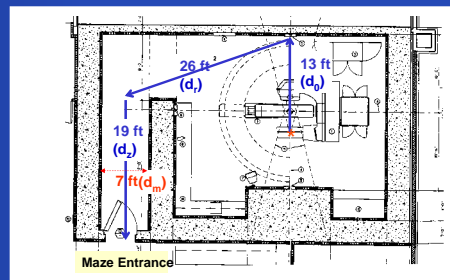


Example 9b: Wall Scatter Unshielded Dose Rate Calculation

Page 109

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	6	
b	W	Workload	Gy/wk	450	
c	f	Patient transmission		0.25	0.25 if MV ≤ 10
d	d _p	Distance from target to primary barrier wall	ft	13	measured
e			m	3.96	d * 0.3048
f	d _p	Distance from primary barrier wall to maze inside opening	ft	26	measured
g			m	7.92	f * 0.3048
h	d _i	Distance from maze inside opening to door	ft	19	measured
i			m	5.79	h * 0.3048
j	d _m	Maze width	ft	7	measured
k			m	2.13	j * 0.3048
l	h	Room height	ft	10	measured
m			m	3.05	L * 0.3048
n	α ₀	1st reflection coefficient	1 / m ²	0.0027	Table 8a with 6 MV 75° scatter angle
o	A ₀	Effective field size	cm	40.0	see above
p	A ₀	Beam area at first reflection	m ²	2.51	(e * o/100)/2
q	α ₂	2nd bounce scatter fraction / m ²		0.0080	Table 8a with 0.5 MV 75° scatter angle
r	A ₂	Maze cross section	m ²	6.5	j * L
s	U	Use Factor		0.25	Orientation with highest dose rate
t	f H _s	Wall scatter unshielded dose rate	mSv/wk	3.00E-04	$\frac{1000 \cdot m^2 \cdot W \cdot f \cdot U \cdot A_0}{(e^2 \cdot g^2 \cdot h^2 \cdot L)}$

Example 9c: Maze with Secondary Leakage Through Door — Leakage Scatter

Page 110

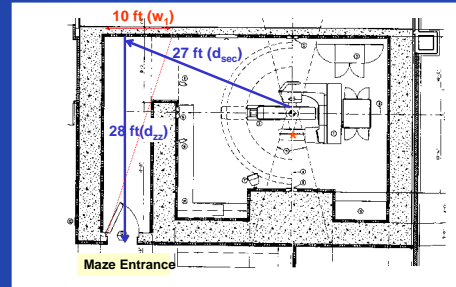

d_{sec} measured from isocenter (the average target location)


Example 9c: Leakage Scatter Unshielded Dose Rate Calculation

Page 111

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	6	
b	W	Workload	Gy/wk	450	
c		Leakage Fraction	%	0.10%	
d		IMRT Factor		2	
e	d _{sec}	Distance from target to wall at maze end	ft	27	measured
f			m	8.23	d * 0.3048
g	d _{2z}	Distance from wall at maze end to door	ft	28	measured
h			m	8.53	f * 0.3048
i	w ₁	Wall width seen from door	ft	10	measured
j			m	3.05	h * 0.3048
k	h	Room height	ft	10	measured
l			m	3.05	j * 0.3048
m	α ₁	1st reflection coefficient	1 / m ²	0.0183	Table 8b with 1.4 MV 0° Reflection angle
n	A ₁	Scatter area	m ²	9.3	i * k
o	U	Use Factor		1	Calculation does not depend on orientation
p	H _{LS}	Leakage scatter unshielded dose rate	mSv/wk	3.10E-02	$\frac{1000 \cdot b \cdot o \cdot c \cdot d \cdot m \cdot n}{(f^2 \cdot h^2)}$

Example 9d: Maze with Secondary Leakage Through Door — Direct Leakage

Page 112

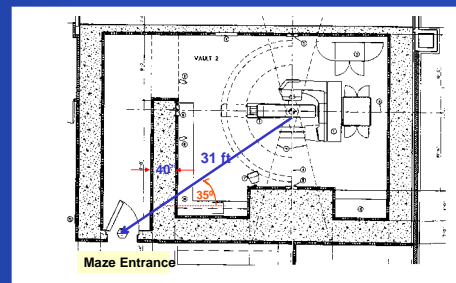

Example 9d: Direct Leakage Unshielded Dose Rate Calculation

Page 113

Line	Parameter	Units	Value	Calculation
a	Machine X-ray Energy	MV	6	
b	Workload (W)	Gy/Wk	450	
c	Use Factor	Ratio	1	
d	Leakage Fraction	%	0.10%	
e	IMRT Factor		2	
f	Isocenter to Protected Point Distance	ft	31.0	
g		m	9.4	f * 0.3048
h	Unshielded Dose Rate	mSv/wk	1.01E+01	$1000 \cdot b \cdot c \cdot d \cdot e / g^2$
i	Wall Transmission		7.86E-05	see below
j	Inside of Door Dose Rate	mSv/wk	7.92E-04	h * i

Barrier	Material Thickness (inches)	Slant Thickness (mm)	Material	Patient Scatter TVL1 (mm)	TVLe (mm)	Photon Trans.
Inside Layer	40	1240	Concrete	340	290	7.86E-05
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 35				6 MV	Total:	7.86E-05

Example 9: Maze Door Transmission Calculation

Page 114

Maze Patient Scatter Transmission for Door						
Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	0.25	6	Lead	5	5	5.37E-02
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 0				0.2 MV	Total:	5.37E-02

Maze Wall Scatter Transmission for Door						
Barrier	Material Thickness		Material	Wall Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	0.25	6	Lead	5	5	5.37E-02
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 0				0.2 MV	Total:	5.37E-02

Maze Leakage Scatter Transmission for Door						
Barrier	Material Thickness		Material	Leakage Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	0.25	6	Lead	8	8	1.61E-01
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 0				0.3 MV	Total:	1.61E-01

Example 9: Maze Door Shielded Dose Rate

Page 115

Maze Direct Leakage Transmission for Door						
Barrier	Material Thickness		Material	Direct Leakage		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	0.25	6	Lead	57	57	7.74E-01
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 0				6 MV	Total:	7.74E-01

Maze Shielded Dose at Door							
Line	Parameter	Units	Patient Scatter	Wall Scatter	Leakage Scatter	Direct Leakage	Calculation
a	Calc. Unshielded Dose Rate	mSv/wk	2.50E-02	3.00E-04	3.10E-02	7.92E-04	
b	Total / Calc. Dose Rate		2.64	2.64	1	1	McGinley
c	Total Unshielded Dose Rate	mSv/wk	6.60E-02	7.92E-04	3.10E-02	7.92E-04	a * b
d	Energy for TVL	MV	0.2	0.2	0.3	6.0	
e	Transmission		5.37E-02	5.37E-02	1.61E-01	7.74E-01	see above
f	Shielded Dose Rate	mSv/wk	0.00354	0.00004	0.00499	0.00061	c * e
g	Total Shielded Dose Rate	mSv/wk			0.0052		Sum Row f

0.0052 mSv/wk is less than
P/T = 0.100 mSv/wk

Example 9: Wall Adjacent to Maze Door Transmission Calculation

Page 116

Maze Patient Scatter Transmission for Wall Adjacent to Door						
Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	6	152	Concrete	130	130	6.73E-02
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle: 0 deg				0.2 MV	Total:	6.73E-02

Maze Wall Scatter Transmission for Wall Adjacent to Door						
Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	6	152	Concrete	130	130	6.73E-02
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle: 0 deg				0.2 MV	Total:	6.73E-02

Maze Leakage Scatter Transmission for Wall Adjacent to Door						
Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	6	152	Concrete	160	160	1.12E-01
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle: 0 deg				0.3 MV	Total:	1.12E-01

Example 9: Wall Adjacent to Maze Door Shielded Dose Rate

Page 117


Maze Direct Leakage Transmission for Wall Adjacent to Door						
Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	6	152	Concrete	340	290	2.98E-01
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle: 0 deg				6 MV	Total:	2.98E-01

Maze Shielded Dose at Wall Adjacent to Door							
Line	Parameter	Units	Patient Scatter	Wall Scatter	Leakage Scatter	Direct Leakage	Calculation
a	Calc. Unshielded Dose Rate	mSv/wk	2.50E-02	3.00E-04	3.10E-02	7.92E-04	
b	Total / Calc. Dose Rate		2.64	2.64	1	1	McGinley
c	Total Unshielded Dose Rate	mSv/wk	6.60E-02	7.92E-04	3.10E-02	7.92E-04	a * b
d	Energy for TVL	MV	0.2	0.2	0.3	6.0	
e	Transmission		6.73E-02	6.73E-02	1.12E-01	2.98E-01	see above
f	Shielded Dose Rate	mSv/wk	0.0044	0.0001	0.0035	0.0002	c * e
g	Total Shielded Dose Rate	mSv/wk			0.0082		Sum Row f

Example 10: Conventional Maze, 18 MV

Page 118

- Same maze layout as Example 1
 - Conventional maze similar to examples in NCRP 151
- Mechanisms included in door calculation
 - Neutron mechanisms dominate shielded dose




- Direct leakage must be calculated
 - With door also contributing to attenuation of direct leakage
- Scatter mechanisms need not be calculated
 - Calculations are included to illustrate that scatter is negligible

Door: 1" lead, 3" borated polyethylene with 0.25" steel covers

Example 10e: Maze with Secondary Leakage Through Door — Maze Neutrons

Page 119

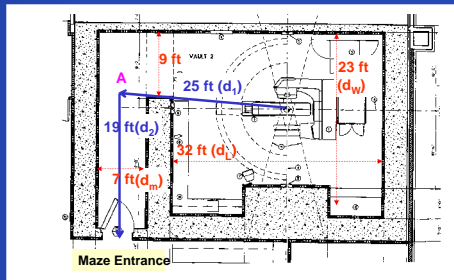

Example 10e: Maze Neutron Fluence Calculation

Page 120

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	18	
b		Vendor		Varian	
c		Neutron IMRT Factor		1	
d	β	Head Transmission Factor		1	1 for lead, 0.85 for tungsten head shield
e	d_i	Distance from isocenter to maze opening (Point A)	ft	25	measured
f			m	7.62	$e * 0.3048$
g	d_L	Vault Average Length	ft	32	measured
h			m	9.75	$g * 0.3048$
i	d_w	Vault Average Width	ft	23	measured
j			m	7.01	$i * 0.3048$
k	h	Vault Average Height	ft	10	measured
L			m	3.05	$k * 0.3048$
m	S_v	Vault Surface Area	m^2	238.9	$2 * (h * j + h * L + j * L)$
n	Q_n	Neutron Source Strength	n / Gy	9.60E+11	Function of a & b
o	Φ_A	Neutron Fluence at Point A per Gy	n / m^2 / Gy	5.60E+09	$c * n * [d / (4 * \pi * r^2) + (5.4 * r + 1.3) / (2 * \pi * m)]$

Example 10e: Capture Gamma Unshielded Dose Rate Calculation

Page 121

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	18	
a	W	Workload	Gy/wk	450	
c	Φ_A	Neutron Fluence at Point A per Gy	n/m ² /Gy	5.60E+09	see above
d	d_z	Distance from maze opening (Point A) to door	ft	19	measured
e	d_0	Inner Maze Entrance Width	m	5.79	$d \cdot 0.3048$
f	TVD	Tenth-Value Distance	m	5.4	3.9 if a<18, 5.4 otherwise
g	K	Ratio Capture Gamma Dose-Equivalent to Neutron Fluence		6.9E-16	Constant
h	h_ϕ	Capture Gamma Unshielded Dose at Door per Dose at Isocenter	Sv/Gy	3.27E-07	$g \cdot c \cdot 10^{(e-f)}$
i	$H_{c\phi}$	Capture Gamma Unshielded Dose Rate	mSv/wk	1.47E-01	$1000 \cdot a \cdot h$


Example 10e: Maze Neutron Unshielded Dose Rate Calculation

Page 122

Line	Symbol	Parameter	Units	Value	Calculation
a	W	Workload	Gy/wk	450	
b	Φ_A	Neutron Fluence at Point A per Gy	n/m ² /Gy	5.60E+09	See above
c	d_z	Distance from maze opening (Point A) to door	ft	19	measured
d	d_0	Inner Maze Entrance Width	m	5.79	$c \cdot 0.3048$
e	d_0	Inner Maze Entrance Width	ft	9	measured
f	d_0	Inner Maze Entrance Width	m	2.74	$e \cdot 0.3048$
g	h	Inner Maze Entrance Height	ft	10	measured
h	h	Inner Maze Entrance Height	m	3.05	$g \cdot 0.3048$
i	S_0	Inner Maze Cross-Sectional Area	m ²	8.36	$f \cdot h$
j	d_m	Maze Width	ft	7	measured
k	d_m	Maze Width	m	2.13	$j \cdot 0.3048$
L	h_m	Average Height Along Maze	ft	10	measured
m	h_m	Average Height Along Maze	m	3.05	$L \cdot 0.3048$
n	S	Maze Cross-Sectional Area	m ²	6.50	$i \cdot m$
o	TVD _n	Maze Neutron Tenth-Value Distance	m	5.25	$2.05 \cdot \text{sqrt}(n)$
p	$H_{n,D}$	Neutron Unshielded Dose-Equivalent at Door per Dose at Isocenter	Sv/Gy	1.23E-06	$2.4E-15 \cdot b \cdot \text{sqrt}(f/n) \cdot (1.64 \cdot 10^{-4} \cdot (d/f) \cdot 9) \cdot 10^4 \cdot (d/f)$
q	H_n	Neutron Unshielded Dose-Equivalent Rate at Door	Sv/wk	5.52E-01	$1000 \cdot a \cdot p$

Example 10a: Maze with Secondary Leakage Through Door — Patient Scatter

Page 123

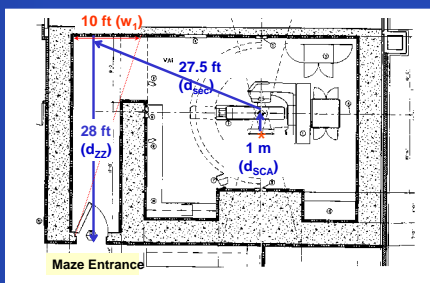

Example 10 P/T and Average Field Size Calculation

Page 124

Line	Parameter	Units	Value	Calculation
a	Machine X-ray Energy	mSv/wk	18	
b	Workload / Treatment	Gy/pt	3	NCRP 151 Default
c	Patients per Day	pt/day	30	NCRP 151 Default
d	Workload (W)	Gy/wk	450	$5 \cdot b \cdot c$
e	Design Dose Limit (P)	mSv/wk	0.1	
f	Occupancy Factor (T)		1	
g	P/T	mSv/wk	0.100	e / f

Line	Parameter	Units	Value		Calculation
			w/o IMRT	with IMRT	
a	Max Field Size	cm	40	40	
b	Fraction of Workload		50%	50%	
c	Effective Field Area	cm ²	1600		$b_1 \cdot a_1^2 + b_2 \cdot a_2^2$
d	Effective Field Size	cm	40.0		$\text{sqrt}(c)$


Example 10a: Patient Scatter Unshielded Dose Rate Calculation

Page 125

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	18	
b	W	Workload	Gy/wk	450	
c	d_{sc}	Distance from target to isocenter	m	1.00	
d	d_{sc}	Distance from isocenter to wall at maze end	ft	27.5	measured
e	d_{sc}	Distance from isocenter to wall at maze end	m	8.38	$d \cdot 0.3048$
f	d_{zz}	Distance from wall at maze end to door	ft	28	measured
g	d_{zz}	Distance from wall at maze end to door	m	8.53	$f \cdot 0.3048$
h	w_1	Wall width seen from door	ft	10	measured
i	w_1	Wall width seen from door	m	3.05	$h \cdot 0.3048$
j	h	Room height	ft	10	measured
k	h	Room height	m	3.05	$j \cdot 0.3048$
L	A_1	Scatter area	m ²	9.3	$i \cdot k$
m	a	Patient scatter fraction (400 cm ² field)		8.64E-04	See Table 5 (45°) Function of MV
n	α_1	2nd bounce scatter fraction / m ²		2.20E-02	Table 8a, 0.5 MV, 45°
o	F	Average field area	cm ²	1600	See above
p	U	Use Factor		0.25	Orientation with highest dose rate
q	H_{ps}	Patient scatter unshielded dose rate	mSv/wk	1.55E-02	$1000 \cdot m \cdot b \cdot p \cdot (c/400)^L / (c^2 \cdot e^2 \cdot g^2)$

Example 10b: Maze with Secondary Leakage Through Door — Wall Scatter

Page 126

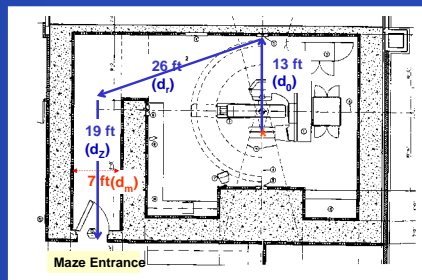


Example 10b: Wall Scatter Unshielded Dose Rate Calculation

Page 127

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	18	
b	W	Workload	Gy/wk	450	
c	f	Patient transmission		0.27	0.27 if MV > 10
d	d _p	Distance from target to primary barrier wall	ft	13	measured
e			m	3.96	d * 0.3048
f	d _i	Distance from primary barrier wall to maze inside opening	ft	26	measured
g			m	7.92	f * 0.3048
h	d _j	Distance from maze inside opening to door	ft	19	measured
i			m	5.79	h * 0.3048
j	d _m	Maze width	ft	7	measured
k			m	2.13	j * 0.3048
L	h	Room height	ft	10	measured
m			m	3.05	L * 0.3048
n	α ₀	1st reflection coefficient	1 / m ²	0.0016	Table 8a with 6 MV 75° scatter angle
o	A ₀	Effective field size	cm	40.0	see above
p	A ₁	Beam area at first reflection	m ²	2.51	(e * o / 100) * 2
q	α _c	2nd bounce scatter fraction / m ²		0.0080	Table 8a with 0.5 MV 75° scatter angle
r	A ₂	Maze cross section	m ²	6.5	j * L
s	U	Use Factor		0.25	Orientation with highest dose rate
s	f H _S	Wall scatter unshielded dose rate	mSv/wk	1.92E-04	1000 * m * s * (0.400) / (e * 2 * g * 2 * i * 2)

Example 10c: Maze with Secondary Leakage Through Door — Leakage Scatter

Page 128

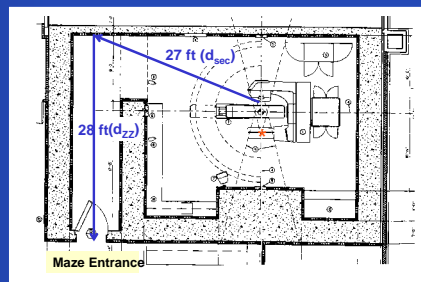


Example 10c: Leakage Scatter Unshielded Dose Rate Calculation

Page 129

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	18	
b	W	Workload	Gy/wk	450	
c		Leakage Fraction	%	0.10%	
d		IMRT Factor		2	
e	d _{sec}	Distance from target to wall at maze end	ft	27	measured
f			m	8.23	d * 0.3048
g	d _{zz}	Distance from wall at maze end to door	ft	28	measured
h			m	8.53	f * 0.3048
i	w ₁	Wall width seen from door	ft	10	measured
j			m	3.05	h * 0.3048
k	h	Room height	ft	10	measured
L			m	3.05	j * 0.3048
m	α ₁	1st reflection coefficient	1 / m ²	0.0179	Table 8b with 1.4 MV 0° Reflection angle
n	A ₁	Scatter area	m ²	9.3	i * k
o	U	Use Factor		1	Calculation does not depend on orientation
p	H _{LS}	Leakage scatter unshielded dose rate	mSv/wk	3.03E-02	1000 * b * o * c * d * m * n / (f * 2 * h * 2)

Example 10d: Maze with Secondary Leakage Through Door — Direct Leakage

Page 130

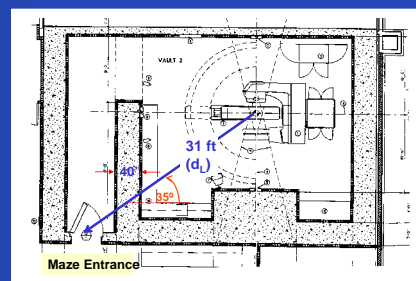

Example 10d: Direct Leakage Unshielded Dose Rate Calculation

Page 131

Line	Parameter	Units	Value	Calculation
a	Machine X-ray Energy	MV	18	
b	Workload (W)	Gy/Wk	450	
c	Use Factor	Ratio	1	
d	Leakage Fraction	%	0.10%	
e	IMRT Factor		2	
f	Isocenter to Protected Point Distance	ft	31.0	
g		m	9.4	f * 0.3048
h	Unshielded Dose	mSv/wk	1.01E+01	1000 * b * c * d * e / g * 2
i	Wall Transmission		2.58E-04	see below
j	Dose at Inside of Door	mSv/wk	2.60E-03	h * i

Barrier	Material Thickness		Material	Direct Leakage		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	40	1240	Concrete	360	340	2.58E-04
Layer #2						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 35				18 MV	Total:	2.58E-04

Example 10: Maze Door Transmission Calculation [1 of 2]

Page 132

Maze Patient Scatter Transmission for Door						
Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	0.25	6	Steel	26	26	5.70E-01
Layer #2	3	76	Borated Poly	322	322	5.90E-01
Layer #3	1	25	Lead	5	5	8.32E-06
Outside Layer	0.25	6	Steel	26	26	5.70E-01
Slant Angle (degrees): 0				0.2 MV	Total:	1.57E-06

Maze Wall Scatter Transmission for Door						
Barrier	Material Thickness		Material	Wall Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	0.25	6	Steel	26	26	5.70E-01
Layer #2	3	76	Borated Poly	322	322	5.90E-01
Layer #3	1	25	Lead	5	5	8.32E-06
Outside Layer	0.25	6	Steel	26	26	5.70E-01
Slant Angle (degrees): 0				0.2 MV	Total:	1.57E-06

Maze Leakage Scatter Transmission for Door						
Barrier	Material Thickness		Material	Leakage Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVL2 (mm)	
Inside Layer	0.25	6	Steel	39	39	6.87E-01
Layer #2	3	76	Borated Poly	396	396	6.42E-01
Layer #3	1	25	Lead	8	8	6.68E-04
Outside Layer	0.25	6	Steel	39	39	6.87E-01
Slant Angle (degrees): 0				0.3 MV	Total:	2.03E-04

Page 133

Example 10: Maze Door Transmission Calculation [2 of 2]

Maze Direct Leakage Transmission for Door

Barrier	Material Thickness		Material	Direct Leakage		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	0.25	6	Steel	96	96	8.59E-01
Layer #2	3	76	Borated Poly	842	842	8.12E-01
Layer #3	1	25	Lead	57	57	3.98E-01
Outside Layer	0.25	6	Steel	96	96	8.59E-01
Slant Angle (degrees): 0				18 MV	Total:	2.15E-01

Neutron Transmission for Door

Barrier	Material Thickness		Material	Maze Neutrons		Neutron Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	0.25	6	Steel	N/A	N/A	1.00E+00
Layer #2	3	76	Borated Poly	45	45	2.03E-02
Layer #3	1	25	Lead	N/A	N/A	1.00E+00
Outside Layer	0.25	6	Steel	N/A	N/A	1.00E+00
Slant Angle (degrees): 0				0.1 MV	Total:	2.03E-02

Capture Gamma Transmission for Door

Barrier	Material Thickness		Material	Capture Gamma		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	0.25	6	Steel	95	95	8.57E-01
Layer #2	3	76	Borated Poly	817	817	8.07E-01
Layer #3	1	25	Lead	61	61	3.93E-01
Outside Layer	0.25	6	Steel	95	95	8.57E-01
Slant Angle (degrees): 0				3.6 MV	Total:	2.27E-01

Page 134

Example 10: Maze Door Shielded Dose Rate

Line	Parameter	Units	Patient Scatter	Wall Scatter	Leakage Scatter	Direct Leakage	Neutrons	Capture Gammas
a	Calc. Unshield Dose Rate	mSv/wk	1.55E-02	1.92E-04	3.03E-02	2.60E-03	5.52E-01	1.47E-01
b	Total / Calc. Dose Rate		2.64	2.64	1	1	1	1
c	Total Unshield Dose Rate	mSv/wk	4.10E-02	5.07E-04	3.03E-02	2.60E-03	5.52E-01	1.47E-01
d	Energy for TVL	MV	0.2	0.2	0.3	18.0	0.1	3.6
e	Transmission		1.57E-06	1.57E-06	2.03E-04	2.15E-01	2.03E-02	2.27E-01
f	Shielded Dose Rate	mSv/wk	0.0000	0.0000	0.0000	0.0006	0.0112	0.0335
g	Total Shielded Dose Rate	mSv/wk				0.0452		

- Shielded dose typically dominated by neutrons and capture gammas
- Direct leakage may be significant or not, depending on maze wall width (not very large in this case)
- Scatter is negligible for high energy
 - Scatter calculation not really required for greater than 10 MV

Page 135

Example 10: Wall Adj. to Maze Door Transmission Calc. [1 of 2]

Maze Patient Scatter Transmission for Wall Adjacent to Door

Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	12	305	Concrete	130	130	4.52E-03
Layer #2						1.00E+00
Layer #3						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 0				0.2 MV	Total:	4.52E-03

Maze Wall Scatter Transmission for Wall Adjacent to Door

Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	12	305	Concrete	130	130	4.52E-03
Layer #2						1.00E+00
Layer #3						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 0				0.2 MV	Total:	4.52E-03

Maze Leakage Scatter Transmission for Wall Adjacent to Door

Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	12	305	Concrete	160	160	1.24E-02
Layer #2						1.00E+00
Layer #3						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 0				0.3 MV	Total:	1.24E-02

Page 136

Example 10: Wall Adj. to Maze Door Transmission Calc. [2 of 2]

Maze Direct Leakage Transmission for Wall Adjacent to Door

Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	12	305	Concrete	360	340	1.27E-01
Layer #2						1.00E+00
Layer #3						1.00E+00
Outside Layer						1.00E+00
Slant Angle: 0 deg				18 MV	Total:	1.27E-01

Neutron Transmission for Wall Adjacent to Door

Barrier	Material Thickness		Material	Patient Scatter		Neutron Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	12	305	Concrete	161	161	1.28E-02
Layer #2						1.00E+00
Layer #3						1.00E+00
Outside Layer						1.00E+00
Slant Angle: 0 deg				0.1 MV	Total:	1.28E-02

Capture Gamma Transmission for Wall Adjacent to Door


Barrier	Material Thickness		Material	Patient Scatter		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	12	305	Concrete	330	330	1.19E-01
Layer #2						1.00E+00
Layer #3						1.00E+00
Outside Layer						1.00E+00
Slant Angle: 0 deg				3.6 MV	Total:	1.19E-01

Page 137

Example 10: Wall Adjacent to Maze Door Shielded Dose Rate

Maze Shielded Dose at Wall Adjacent to Door

Line	Parameter	Units	Patient Scatter	Wall Scatter	Leakage Scatter	Direct Leakage	Neutrons	Capture Gammas	Calculation
a	Calc. Unshield Dose Rate	mSv/wk	1.55E-02	1.92E-04	3.03E-02	2.60E-03	5.52E-01	1.47E-01	
b	Total / Calc. Dose Rate		2.64	2.64	1	1	1	1	NCRP 151 Eq. 2.14
c	Total Unshield Dose Rate	mSv/wk	4.10E-02	5.07E-04	3.03E-02	2.60E-03	5.52E-01	1.47E-01	a * b
d	Energy for TVL	MV	0.3	0.3	0.5	18.0	0.1	3.6	
e	Transmission		4.52E-03	4.52E-03	1.24E-02	1.27E-01	1.28E-02	1.19E-01	see above
f	Shielded Dose Rate	mSv/wk	0.0002	0.0000	0.0004	0.0003	0.0071	0.0175	c * e
g	Total Shielded Dose Rate	mSv/wk				0.0255			Sum Row f

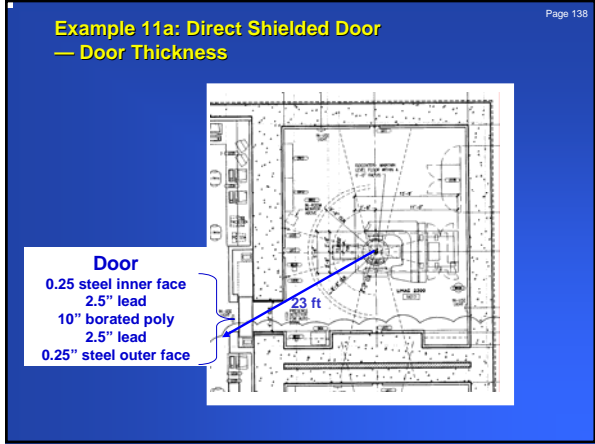

Example 11a: Direct Shielded Door Thickness Calculation [1 of 2]

Page 139

Line	Parameter	Units	Value	Calculation
a	Design Dose Limit (P)	mSv/wk	0.1	
b	Occupancy Factor (T)		1	
c	P/T	mSv/wk	0.100	a / b
d	Machine X-ray Energy	MV	18	
e	Vendor		Varian	

Line	Parameter	Units	Value		Calculation
			w/o IMRT	with IMRT	
a	Max Field Size	cm	40	40	
b	Fraction of Workload		50%	50%	
c	Effective Field Area	cm ²	1600.0	1600.0	$b_1 \cdot a_1^2 + b_2 \cdot a_2^2$
d	Effective Field Size	cm	40.0	40.0	$\text{sqrt}(c)$
e	Scatter Angle	deg	60	60	
f	Machine X-ray Energy	MV	18	18	
g	Scatter / 400 cm ²		4.24E-04	4.24E-04	Function of e & f
h	Scatter Fraction		0.00170	0.00170	$g \cdot c / 400$

Example 11a: Direct Shielded Door Thickness Calculation [2 of 2]


Page 140

Line	Parameter	Units	Photon Leakage	Photon Scatter	Neutron Leakage	Calculation
a	Workload / Treatment	Gy/pt	3	3	3	NCRP 151 default
b	Patients per Day	pt/day	30	30	30	NCRP 151 default
c	Workload (W)	Gy/wk	450	450	450	$5 \cdot a \cdot b$
d	Use Factor	Ratio	1	1	1	
e	Fraction		1.00E-03	1.70E-03	1.5E-03	18 MV values
f	IMRT Factor		2	1	1	
g	Isocenter to Protected Point Distance	ft	23.0	23.0	23.0	
h	Isocenter to Protected Point Distance	m	7.0	7.0	7.0	$g \cdot 0.3048$
i	Unshielded Dose Rate	mSv/wk	1.83E+01	1.55E+01	1.37E+01	$1000 \cdot c \cdot d \cdot e \cdot f \cdot h^2$
j	Transmission		8.44E-04	8.44E-07	8.81E-04	see below
k	Shielded Dose Rate	mSv/wk	0.0154	0.0000	0.0121	$i \cdot j$
L	Total Shielded Dose Rate	mSv/wk		0.0276		Sum row k

Barrier	Material	Thickness	Photon Leakage		Scatter		Neutron				
			TVL1 (mm)	TVLc (mm)	TVL1 (mm)	TVLc (mm)	TVL (mm)	Trans.			
Inside Layer	0.25	7	Steel	96	8.39E-01	68	68	7.80E-01	N/A	1.00E+00	
Layer #2	2.5	73	Lead	57	5.17E-02	32	32	5.11E-03	N/A	1.00E+00	
Layer #3	10	293	Borated Poly	891	842	4.48E-01	230	230	5.31E-02	96	8.81E-04
Layer #4	2.5	73	Lead	57	5.17E-02	32	32	5.11E-03	N/A	1.00E+00	
Outside Layer	0.25	7	Steel	96	8.39E-01	68	68	7.80E-01	N/A	1.00E+00	
Slant Angle (degrees):	30		18 MV		Total:	8.44E-04	Total:	8.44E-07	Total:	8.81E-04	


Example 11b: Direct Shielded Door — Additional Shielding for Far Side of Door

Page 141

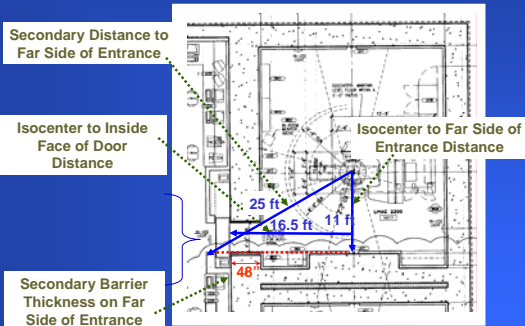


Example 11b: Direct Shielded Door — Additional Shielding for Far Side of Door

Page 142

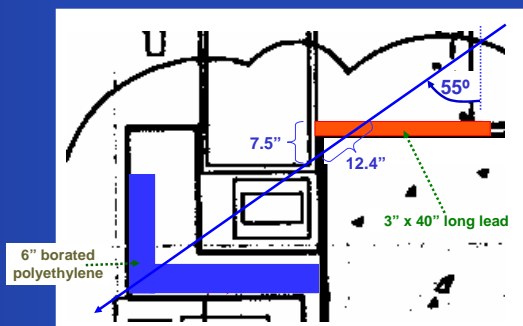

Example 11b: Direct Shielded Door — Additional Shielding for Far Side of Door

Page 143

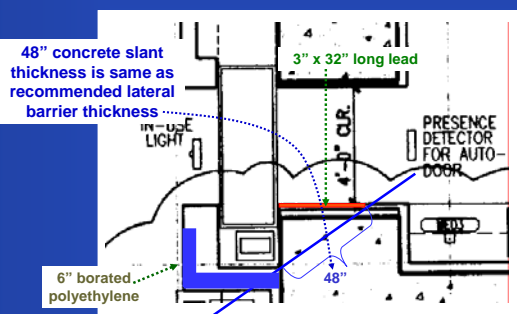

Example 11b: Direct Shielded Door Far Side of Entrance Shielded Dose Rate Calculation [1 of 3]

Page 144

Line	Parameter	Units	Value	Calculation
a	Door Overlap	in	7.5	
b	Gap Between Barrier and Door	in	0.5	
c	Distance from Isocenter to Far Side of Entrance	ft	11	
d	Distance from Isocenter to Inside Face of Door	ft	16.5	$c \cdot 12$
e	Slant Angle at Far Side of Entrance	deg	54.8	$\text{atan}(f / (a + d))$
f	Slant Thickness at Corner	in	12.4	$a / \cos(g) - b / \sin(g)$
g	Thickness of Lead Added to Wall	in	3	Selected value
h	Slant Thickness through Lead	mm	132	$25.4 \cdot j / \cos(g)$
i	Slant Thickness through Concrete	in	183	$i - k$
j	Concrete Thickness	in	4.15	$L \cdot \cos(g) / 25.4$
k	Borated Poly Thickness	in	6	Selected value
l	Borated Poly Slant Thickness	mm	186	$25.4 \cdot n / \sin(g)$
m	Minimum Desired Slant Thickness	in	42	Dose rate < P/T / 3
n	Minimum Length of Added Lead	in	35	$p \cdot \sin(g)$

- Thicknesses selected to make shielded dose rate less than dose limit

Example 11b: Direct Shielded Door Far Side of Entrance Shielded Dose Rate Calculation [2 of 3]

Far Side of Door Scatter Fraction Calculation


Line	Parameter	Units	Value		Calculation
			w/o IMRT	with IMRT	
a	Max Field Size	cm	40	40	
b	Fraction of Workload		50%	50%	
c	Effective Field Area	cm ²	1600.0		$b \cdot a_1^2 + b \cdot a_2^2$
d	Effective Field Size	cm	40.0		sqrt (c)
e	Scatter Angle	deg	54.8		
f	Machine X-ray Energy	MV	18		
g	Scatter / 400 cm ²		5.42E-04		Function of e & f
h	Scatter Fraction		0.00217		$g \cdot c / 400$

Example 11b: Direct Shielded Door Far Side of Entrance Shielded Dose Rate Calculation [3 of 3]


Line	Parameter	Units	Photon Leakage	Photon Scatter	Neutron Leakage	Calculation
a	Workload / Treatment	Gy/pt	3	3	3	NCRP 151 default
b	Patients per Day	pt/day	30	30	30	NCRP 151 default
c	Workload (W)	Gy/wk	450	450	450	$5 \cdot a \cdot b$
d	Use Factor	Ratio	1	1	1	
e	Fraction		1.00E-03	2.17E-03	1.50E-03	18 MV values
f	IMRT Factor		2	1	1	
g	Isocenter to Protected Point Distance	ft	25.0	25.0	25.0	
h		m	7.6	7.6	7.6	$g \cdot 0.3048$
i	Unshielded Dose	mSv/wk	1.55E+01	1.68E+01	1.16E+01	$1000 \cdot c \cdot d \cdot e \cdot f \cdot h^2$
j	Transmission		8.31E-04	6.14E-06	1.55E-03	see below
k	Shielded Dose	mSv/wk	0.013	0.000	0.018	$i \cdot j$
L	Total Shielded Dose	mSv/wk		0.031		Sum row k

Barrier	Material Thickness	Slant Thickness	Material	Photon Leakage			Scatter			Neutron		
				TVL1 (mm)	TVLc (mm)	Trans.	TVL1 (mm)	TVLc (mm)	Trans.	TVL (mm)	Trans.	
Inside Layer	3	132	Lead	57	57	4.77E-03	36	36	2.01E-04	N/A	1.00E+00	
Layer #2	4.1	183	Concrete	360	340	2.90E-01	244	244	1.78E-01	211	1.38E-01	
Layer #3	6	196	Borated Poly	891	842	6.01E-01	244	244	1.72E-01	96	1.14E-02	
Layer #4						1.00E+00			1.00E+00		1.00E+00	
Outside Layer						1.00E+00			1.00E+00		1.00E+00	
Slant Angle (degrees)	54.8			18 MV			Total:	8.31E-04		Total:	6.14E-06	
							Total:	1.55E-03		Total:	1.55E-03	


Example 11c: Direct Shielded Door— Additional Shielding for Near Side of Door (Wall Scatter)

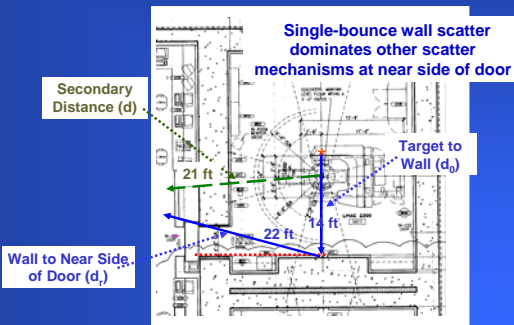


Example 11c: Direct Shielded Door— Additional Shielding for Near Side of Door (Neutrons / Capture Gammas)

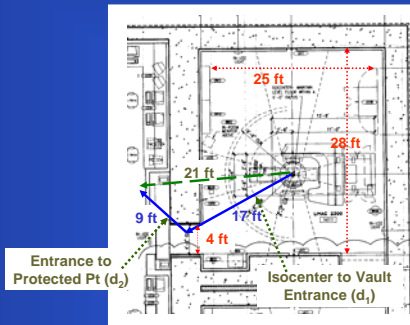

Example 11c: Direct Shielded Door — Gap Between Wall and Door

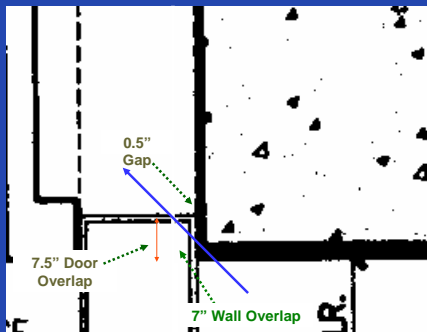

Example 11c: Direct Shielded Door — Additional Shielding for Near Side of Door

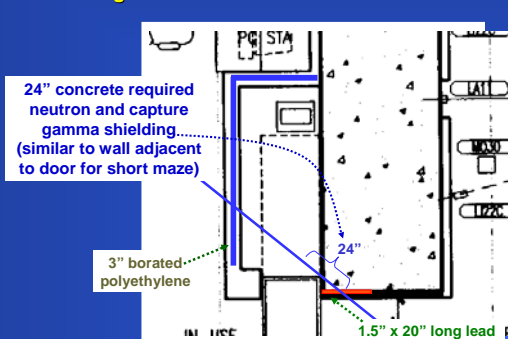

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [1 of 9]

Near Side of Door Material Thickness Calculation

Line	Parameter	Units	Value	Calculation
a	Door Overlap	in	7.5	
b	Gap Between Barrier and Door	in	0.5	
c	Angle at Near Side Wall	deg	45.0	
d	Wall Overlap Beyond Entrance	in	7.0	$(a \cdot \tan(c) - b) / \tan(c)$
e	Thickness of Lead Added to Wall	in	1.5	
f	Remaining Concrete Wall	in	5.5	d - e
g	Material Added beyond Wall	in	3	

- Material added to wall selected as required to make shielded dose rate less than dose limit

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [2 of 9]

Near Side of Door Scatter Fraction Calculation

Line	Parameter	Units	Value		Calculation
			w/o IMRT	with IMRT	
a	Max Field Size	cm	40	40	
b	Fraction of Workload		50%	50%	
c	Effective Field Area	cm ²	1600.0		$b_1 \cdot a_1^2 + b_2 \cdot a_2^2$
d	Effective Field Size	cm	40.0		sqrt (c)
e	Scatter Angle	deg	85		
f	Machine X-ray Energy	MV	18		
g	Scatter / 400 cm ²		2.16E-04		Function of e & f
h	Scatter Fraction		0.00086		$g \cdot c / 400$

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [3 of 9]

Near Side of Door Shielded Dose Due to Direct Leakage

Line	Parameter	Units	Photon Leakage	Photon Scatter	Neutron Leakage	Calculation
a	Workload / Treatment	Gy/pt	3	3	3	NCRP 151 default
b	Patients per Day	pt/day	30	30	30	NCRP 151 default
c	Workload (W)	Gy/wk	450	450	450	$5 \cdot a \cdot b$
d	Use Factor	Ratio	1	1	1	
e	Fraction		1.00E-03	8.65E-04	1.50E-03	18 MV values
f	IMRT Factor		2	1	1	
g	Isocenter to Protected Point Distance	ft	21.0	21.0	21.0	
h		m	6.4	6.4	6.4	$g \cdot 0.3048$
i	Unshielded Dose	mSv/wk	2.20E+01	9.50E+00	1.65E+01	$1000 \cdot c \cdot d \cdot e \cdot f \cdot h^2$
j	Transmission		2.88E-04	5.99E-07	1.58E-06	see below
k	Shielded Dose	mSv/wk	0.006	0.000	0.000	$i \cdot j$
L	Total Shielded Dose	mSv/wk		0.006		Sum row k

Transmission Calculation for Direct Leakage at Near Side of Door

Barrier	Material Thickness		Photon Leakage			Scatter			Neutron			
	Inches	mm	TVL1 (mm)	TVLs (mm)	Trans.	TVL1 (mm)	TVLs (mm)	Trans.	TVL1 (mm)	TVLs (mm)	Trans.	
Inside Layer	48	1224	Concrete	360	340	2.88E-04	197	197	5.99E-07	211	1.58E-06	
Layer #2						1.00E+00			1.00E+00		1.00E+00	
Outside Layer						1.00E+00			1.00E+00		1.00E+00	
Slant Angle (degrees):			5			18 MV	Total:	2.88E-04	Total:	5.99E-07	Total:	1.58E-06

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [4 of 9]

Wall Scatter Transmission for Near Side of Door

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	18	
b	W	Workload	Gy/wk	450	
c	f	Patient transmission		0.27	0.27 if MV ≥ 10
d	d ₀	Distance from target to primary barrier wall	ft	25	measured
e			m	7.62	$d \cdot 0.3048$
f	d _i	Distance from primary barrier wall to near side of maze entrance	ft	9	measured
g			m	2.74	$f \cdot 0.3048$
h	α _c	Reflection coefficient	1 / m ²	0.0016	Table 8a with 18 MV 85° scatter angle
i		Effective field size	cm	40.0	see above
j	A ₀	Beam area at far maze wall	m ²	9.29	$(e \cdot i / 100)^2$
k	U	Use Factor		0.25	Orientation with highest dose rate.
L	f H _S	Wall scatter unshielded dose	mSv/wk	1.03E+00	$1000 \cdot b \cdot c \cdot k \cdot h \cdot j / (e^2 \cdot g^2)$

Near Side of Door Wall Scatter Transmission Calculation

Barrier	Material Thickness		Wall Scatter		Photon Trans.
	Inches	mm	Material	TVL1 (mm) / TVLs (mm)	
Inside Layer	1.5	54	Lead	8 / 8	1.84E-07
Layer #2	5.5	198	Concrete	160 / 160	5.82E-02
Layer #3	3	108	Borated Poly	396 / 396	5.34E-01
Slant Angle (degrees):			45		
				0.3 MV	Total:
					5.73E-09

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [5 of 9]

Maze Neutron Fluence Calculation

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	18	
b	Vendor			Varian	
c		Neutron IMRT Factor		1	
d	β	Head Transmission Factor		1	1 for lead, 0.85 for tungsten head shield
e	d _i	Distance from isocenter to maze opening (Point A)	ft	17	measured
f			m	5.18	$e \cdot 0.3048$
g	d _L	Vault Average Length	ft	28	measured
h			m	8.53	$g \cdot 0.3048$
i	d _w	Vault Average Width	ft	25	measured
j			m	7.62	$i \cdot 0.3048$
k	h	Vault Average Height	ft	10	measured
L			m	3.05	$k \cdot 0.3048$
M	S _v	Vault Surface Area	m ²	228.5	$2 \cdot (h \cdot j) + h \cdot L + j \cdot L$
n	Q _n	Neutron Source Strength	n / Gy	9.60E+11	Function of a & b
o	Φ _A	Neutron Fluence at Point A per Gy	n / m ² / Gy	7.32E+09	$c \cdot n \cdot [1 / (d_i^2 \cdot f^2) + (5.4 \cdot d_i + 1.3) / (2 \cdot g \cdot m)]$

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [6 of 9]

Capture Gamma Unshielded Dose Rate Calculation

Line	Symbol	Parameter	Units	Value	Calculation
a	MV	Machine X-ray Energy	MV	18	
b	W	Workload	Gy/wk	450	
c	Φ _A	Neutron Fluence at Point A per Gy	n / m ² / Gy	7.32E+09	see above
d	d ₂	Distance from maze opening (Point A) to door	ft	9	measured
e			m	2.74	$d \cdot 0.3048$
f	TVD	Tenth-Value Distance	m	5.4	3.9 if a < 18, 5.4 otherwise
g	K	Ratio Capture Gamma Dose-Equivalent to Neutron Fluence		6.90E-16	Constant
h	h _p	Capture Gamma Unshielded Dose at Door per Dose at Isocenter	Sv/Gy	1.57E-06	$g \cdot c \cdot 10^4 \cdot (e / f)$
i		Capture Gamma Unshielded Dose Rate	mSv/wk	7.06E-01	$1000 \cdot a \cdot h$

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [7 of 9]

Maze Neutron Unshielded Dose-Equivalent Calculation (Modified Kersey Method)					
Line	Symbol	Parameter	Units	Value	Calculation
a	W	Workload	Gy/wk	450	
b	Φ_A	Neutron Fluence at Point A per Gy	n/m ² /Gy	7.32E+09	See above
c	d_2	Distance from maze opening (Point A) to door	ft	9	measured
d			m	2.74	c * 0.3048
e	d_0	Inner Maze Entrance Width	ft	4	measured
f			m	1.22	e * 0.3048
g	h	Inner Maze Entrance Height	ft	10	measured
h			m	3.05	g * 0.3048
i	S_0	Inner Maze Cross-Sectional Area	m ²	3.72	f * h
j	d_m	Maze Width	ft	4	measured
k			m	1.22	j * 0.3048
L	h_m	Average Height Along Maze	ft	10	measured
m			m	3.05	L * 0.3048
n	S	Maze Cross-Sectional Area	m ²	3.72	i * m
o	TVD_n	Maze Neutron Tenth-Value Distance	m	3.97	$2.06 * \sqrt{\text{sq}(n)}$
p	$H_{n,D}$	Neutron Unshielded Dose-Equivalent at Door per Dose at Isocenter	Sv/Gy	4.62E-06	$2.4E-15 * b * \sqrt{\text{sq}(i/n) * [1.64^{10} * (d/d_0)^2]}$
q		Neutron Unshielded Dose-Equivalent Rate at Door	Sv/wk	2.08E+00	$1000 * a * p$

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [8 of 9]

Neutron Transmission for Near Side of Maze Entrance						
Barrier	Material Thickness	Slant Thickness	Material	Neutrons		Neutron Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	1.5	54	Lead	1000000	1000000	1.00E+00
Layer #2	5.5	198	Concrete	161	161	5.93E-02
Layer #3	3	108	Borated Poly	45	45	4.03E-03
Layer #4						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 45					0.1 MV	Total: 2.39E-04

Capture Gamma Transmission for Near Side of Maze Entrance						
Barrier	Material Thickness	Slant Thickness	Material	Capture Gammas		Photon Trans.
	inches	mm		TVL1 (mm)	TVLe (mm)	
Inside Layer	1.5	54	Lead	61	61	1.31E-01
Layer #2	5.5	198	Concrete	410	370	3.01E-01
Layer #3	3	108	Borated Poly	1015	916	7.63E-01
Layer #4						1.00E+00
Outside Layer						1.00E+00
Slant Angle (degrees): 45					10 MV	Total: 3.00E-02

Example 11c: Direct Shielded Door Near Side of Entrance Shielded Dose Rate Calculation [9 of 9]

Maze Shielded Dose at Door						
Line	Parameter	Units	Wall Scatter	Direct Leakage	Neutrons	Capture Gammas
a	Calc. Unshielded Dose	mSv/wk	1.03E+00	6.36E-03	2.08E+00	7.06E-01
b	Total / Calc. Dose Rate		2.64	1	1	1
c	Unshielded Dose Rate	mSv/wk	2.73E+00	6.36E-03	2.08E+00	7.06E-01
b	Energy for TVL	MV	0.3	18	0.1	10.0
c	Transmission		5.73E-09	1.00E+00	2.39E-04	3.00E-02
d	Shielded Dose	mSv/wk	0.0000	0.0064	0.0005	0.0212
e	Total Shielded Dose	mSv/wk			0.0281	